

DATAMASTER DMT MAINTENANCE LOG

Shelburne PD

Department/Agency

100133

DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
12/2/11	DataMaster Simulator Solution Lot # 12-45-100 EtOH_{aq} Conc: 0.100 Range: 0.095 - 0.105 Preparation Date: 12/12/2011 Expires: 12/12/2012 [For RPC or Simulator Solution Change Place Label Here] OPENED: 12/2/11 <i>SK</i> Installation according to Protocol <i>SK 12/2/11</i>	<i>Kirk Kimball</i> <i>VDHL</i> <i>Prog chief.</i>
1/5/12	[For RPC or Simulator Solution Change Place Label Here] Monthly check Supervisor	<i>P. King</i>
2/6/12	DataMaster Simulator Solution Lot # 12-45-100 EtOH_{aq} Conc: 0.100 Range: 0.095 - 0.105 Preparation Date: 12/12/2011 Expires: 12/12/2012 [For RPC or Simulator Solution Change Place Label Here] OPENED: 2-6-12 Routine Performance Check	<i>P. King</i>
3/12/12	DataMaster Simulator Solution Lot # 12-45-100 EtOH_{aq} Conc: 0.100 Range: 0.095 - 0.105 Preparation Date: 12/12/2011 Expires: 12/12/2012 [For RPC or Simulator Solution Change Place Label Here] OPENED: 3/12/12	<i>P. King</i>
4/3/12	TSI Replaced Sim w/ S/N 67454 Adjusted temp. on DMT to Sim	<i>A. Bolduc</i>

DATAMASTER DMT MAINTENANCE LOG

Shelburne P.D

Department/Agency

100133

DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
4/19/12	Monthly Check - OK [For RPC or Simulator Solution Change Place Label Here]	P. King
5/1/12	Monthly check - OK [For RPC or Simulator Solution Change Place Label Here]	P. King
5/26	Sim solution change-out & Range [For RPC or Sim <u>DataMaster Simulator Solution</u> Here] Lot # 12-70-100 EtOHaq Conc: 0.100 Range: 0.095 - 0.105 Preparation Date: 04/17/2012 Expires: 04/17/2013 OPENED: Complete RPC Rin Juice	P. King
6/7/12	Software update [For RPC or Simulator Solution Change Place Label Here] and lock change	Seb

DATAMASTER DMT MAINTENANCE LOG

Shelburne R.D.
Department/Agency

100133
DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
7/8/12	DataMaster Simulator Solution Lot # 12-70-100 EtOH_{aq} Conc: 0.100 Range: 0.095 - 0.105 Preparation Date: 04/17/2012 Expires: 04/17/2013 [For R] Place Label Here] OPENED: 7/6/12 2 Failed test	K. V.
7/6/12	DataMaster Simulator Solution Lot # 12-58-100 EtOH_{aq} Conc: 0.100 Range: 0.095 - 0.105 Preparation Date: 02/09/2012 Expires: 02/09/2013 OPENED: 7-6-12	K. V.
8/1/12	DataMaster Simulator Solution Lot # 12-64-100 EtOH_{aq} Conc: 0.101 Range: 0.096 - 0.106 Preparation Date: 02/17/2012 Expires: 02/17/2013 [For RPC] Place Label Here] OPENED: 8/1/12	K. V.
8/1/12	Monthly check	
	[For RPC or Simulator Solution Change Place Label Here]	
8/8/12	Ran Accuracy & precision test, solution looks good so re-ran sim solution change protocol	R. Driscoll
9/17/12	DataMaster Simulator Solution Lot # 12-77-100 EtOH_{aq} Conc: 0.099 Range: 0.094 - 0.104 Preparation Date: 05/08/2012 Expires: 05/08/2013 [For] Place Label Here] OPENED: 9/12/12 Monthly Check	P. K.

DATAMASTER DMT MAINTENANCE LOG

Shelburne

Department/Agency

102133

DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
10/07/12	<u>DataMaster Simulator Solution</u> Lot # 12-80-100 EtOHaq Conc: 0.099 Range: 0.094 - 0.104 Preparation Date: 07/5/2012 Expires: 7/5/2013 OPENED: 10/7/12 RPC [For RPC or Simulator Solution Change Place Label Here]	R. King
10/9/12	SET RFI SENSATIVITY + RE-Ran RPC Passed!	R. Driscoll
10/30/12	Flow rate was running at upper limit $\approx 6.5 \text{ L/min}$ [For RPC or Simulator Solution Change Place Label Here] Causing "diagnostic check fails". Installed adjustable flow rate valve and set to 1.5L.	R. Driscoll
11/06/12	[For RPC or Simulator Solution Change Place Label Here] APM Protocol performed	R. Driscoll
11/17/12	<u>DataMaster Simulator Solution</u> Lot # 12-84-100 EtOHaq Conc: 0.101 Range: 0.096 - 0.106 Preparation Date: 9/24/2012 Expires: 9/24/2013 OPENED: 11/17/12 [For RPC or Simulator Solution Change Place Label Here] Monthly Report	R. King

DATAMASTER DMT MAINTENANCE LOG

Sherburne

Department/Agency

100133

DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
12/14/12	DataMaster Simulator Solution Lot # 12-80-100 EtOHaq Conc: 0.099 Range: 0.094 - 0.104 Preparation Date: 07/5/2012 Expires: 7/5/2013 [For RF] Place Label Here] OPENED: 12/14/12 Monthly check	RKF
12/28/12	RAN Accuracy + precision check - checked OK [For RPC or Simulator Solution Change Place Label Here]	J. Munn
1/2/13	DataMaster Simulator Solution Lot # 12-88-100 EtOHaq Conc: 0.098 Range: 0.093 - 0.103 Preparation Date: 11/9/2012 Expires: 11/9/2013 [For RPC or] Label Here] OPENED: 1/2/13 King Monthly check	P. King
2/22/13	DataMaster Simulator Solution Lot # 12-88-100 EtOHaq Conc: 0.098 Range: 0.093 - 0.103 Preparation Date: 11/9/2012 Expires: 11/9/2013 [For RPC] Label Here] OPENED: 2/22/13 MARCOX RAN MONTHLY Check	J. Marcano

DATAMASTER DMT MAINTENANCE LOG

Shelburne P.D.

Department/Agency

100133

DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
March Envy 4/20/13	[For RPC or Simulator Solution Change Place Label Here] Reports to S.H.	P. King
4/27/13	DataMaster Simulator Solution Lot # 13-03-100 EtOHaq Conc: 0.098 Range: 0.093 - 0.103 Preparation Date: 04/03/2013 Expires: 04/03/2014 [For R OPENED: 4-27 KING Monthly check	P. King
6/30/13	DataMaster Simulator Solution Lot # 13-03-100 EtOHaq Conc: 0.098 Range: 0.093 - 0.103 Preparation Date: 04/03/2013 Expires: 04/03/2014 [For RPC OPENED: 6/24/13 RPC Monthly check - Reports TRAP & 14 days Reports	P. King
8/1/13	Monthly check for June & July [For RPC or Simulator Solution Change Place Label Here]	P. King

DATAMASTER DMT MAINTENANCE LOG

Shelburne P.D.
Department/Agency

100133
DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
	[For RPC or Simulator Solution Change Place Label Here]	
9/14	Monthly Inspection	P. Hy
10/8/13	DataMaster Simulator Solution Lot # 13-03-100 EtOHaq Conc: 0.098 Range: 0.093 - 0.103 Preparation Date: 04/03/2013 Expires: 04/03/2014 OPENED: 10/6/13 P. Hy place Label Here] RPC	P. Hy
10/10/13	Wrong Lot # entered during RPC on 10/6/13 [For RPC or Simulator Solution Change Place Label Here] Performed solution change protocol to assign the correct Simulator Solution to the DMT. Checked reports for any effected tickets. RCD 10/10/13	R. Driscoll DMT TECH.
11/15/13	Completed APM Protocol [For RPC or Simulator Solution Change Place Label Here]	R. Driscoll DMT TECH.

DATAMASTER DMT MAINTENANCE LOG

Shelburne P.D.
Department/Agency

100133
DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
12/18/13	[For RPC or Simulator Solution Change Place Label Here] Monthly check	King
1/1/14	<u>DataMaster Simulator Solution</u> Lot # 13-16-100 EtOHaq Conc: 0.099 Range: 0.094 - 0.104 Preparation Date: 9/26/2013 Expires: 09/26/2014 [For RPC or Simulator Solution Change Place Label Here] OPENED: 1-1-14 PK Monthly check	P.K.
2/8/14	<u>DataMaster Simulator Solution</u> Lot # 13-16-100 EtOHaq Conc: 0.099 Range: 0.094 - 0.104 Preparation Date: 9/26/2013 Expires: 09/26/2014 [For RPC or Simulator Solution Change Place Label Here] OPENED: 2/8 R.H. Routine Performance Check	P.H.
3/01	[For RPC or Simulator Solution Change Place Label Here] conducted Accuracy + Precision Report after 5 runs of "SIMULATOR OUT OF RANGE" during SUBJECT SAMPLING.	






DATAMASTER DMT MAINTENANCE LOG

Shelburne P.D.

Department/Agency

100133

DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
	[For RPC or Simulator Solution Change Place Label Here]	
3/1	RAN DUI SUBJECT TEST simulator upon w/i range	
3/8	[For RPC or Simulator Solution Change Place Label Here]	
	Monthly check & solution change	
3/8	DataMaster Simulator Solution Lot # 13-16-100 EtOHaq Conc: 0.099 Range: 0.094 - 0.104 Preparation Date: 9/26/2013 Expires: 09/26/2014 OPENED: 3/8/14  [For RPC or Simulator Solution Change Place Label Here]	
	[For RPC or Simulator Solution Change Place Label Here]	
3/21 0230	complaint of locked screen from prev. night turned off machine, waited a minute, then turned back on; correct screen appeared.	

DATAMASTER DMT MAINTENANCE LOG

Shelburne PD

Department/Agency

100133

DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
3/24/14	DataMaster Simulator Solution Lot # 14-01-100 EtOHaq Conc: 0.099 Range: 0.094 - 0.104 Preparation Date: 1/9/2014 Expires: 1/9/2015 [For RPC e Label Here] OPENED: 3/24/14 RCD DMT supervisor experiencing higher than normal simulator solution usage. Found simulator leaking. Replaced simulator, matched temps and completed solution change.	R. Driscoll DMT TECH
4/5/14	[For RPC or Simulator Solution Change Place Label Here] Monthly Check of Reports	P. Key
6/8/14	DataMaster Simulator Solution Lot # 14-01-100 EtOHaq Conc: 0.099 Range: 0.094 - 0.104 Preparation Date: 1/9/2014 Expires: 1/9/2015 [For RPC e Label Here] OPENED: 6/8/14 Solution change / RPC - During accuracy + precision test, Avg was NOT ± 5%. checked connections, threading, and inspected O-ring. Ran RPC Again - Passed.	J. MARCOW DMT SUPERVISOR
6/23/14 OHS	[For RPC or Simulator Solution Change Place Label Here] Officer Adv'd of INSTRUCTOR when APPROX 10 min test, showed simulator out of range; test removed SUBJECT FROM AREA + obtained a proper breath test; on 2nd test requested, again showed simulator out of range.	J. MARCOW DMT SUPERVISOR

ran accuracy + precision test - passed.



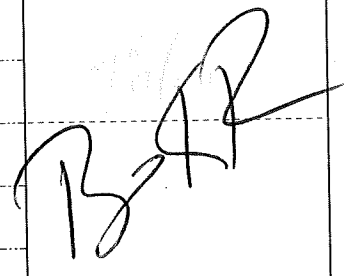
DATA MASTER DMT MAINTENANCE LOG

Shelburne Police

Department/Agency

100133

DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
7/5	[For RPC or Simulator Solution Change Place Label Here] Simulator out of service TOOK OUT OF SERVICE	 DMT Supervisor
7/7	DataMaster Simulator Solution Lot # 14-01-100 EtOHaq Conc: 0.099 Range: 0.094 - 0.104 Preparation Date: 1/9/2014 Expires: 1/9/2015 [For RPC or Simulator Solution Change Place Label Here] OPENED: 5 MAR 2014 IN SERVICE FOR A&P check - failed conducted solution change	 DMT Supervisor
10/14	[For RPC or Simulator Solution Change Place Label Here] DataMaster Simulator Solution Lot # 14-05-100 EtOHaq Conc: 0.098 Range: 0.093 - 0.103 Preparation Date: 6/19/2014 Expires: 6/19/2015 OPENED: RPC OUT	 R. Driscoll DMT Tech.
11/14/14	Completed AEM Protocol [For RPC or Simulator Solution Change Place Label Here]	R. Driscoll DMT Tech.

DATAMASTER DMT MAINTENANCE LOG

She/Burne PD
Department/Agency

100133
DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
2/28/15	DataMaster Simulator Solution Lot # 14-12-100 EtOHaq Conc: 0.098 Range: 0.093 - 0.103 Preparation Date: 9/10/2014 Expires: 9/10/2015 [For R <u>Burne PD 2/28/15</u>] Printer Ink cartridges changed	BRF DMT Supervisor
6/28/15	DataMaster Simulator Solution Lot # 14-12-100 EtOHaq Conc: 0.098 Range: 0.093 - 0.103 Preparation Date: 9/10/2014 Expires: 9/10/2015 [For RP(<u>6/28/15 Burne PD</u>] RPC	BRF DMT Supervisor
10/18/15	[For RPC or Simulator Solution Change Place Label Here] DataMaster Simulator Solution Lot # 15-07-100 EtOHaq Conc: 0.100g/210L Range: 0.095 - 0.105 Preparation Date: 5/11/2015 Expires: 5/11/2016 [<u>Burne PD 10/18/15</u>] RPC	BRF DMT SUP
10/20/15	Completed API protocol, Uploaded new software [For RPC or Simulator Solution Change Place Label Here] downloaded data to USB drive, installed new F/O PCB. Not connected to DES server as there are no available ports. Also adjusted clock ahead 13 minutes to the correct time.	R. Driscoll DMT Tech.

DATAMASTER DMT MAINTENANCE LOG

Department/Agency

DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
2/7/16	[For RPC or Simulator Solution Change Place Label Here] DataMaster Simulator Solution Lot # 15-07-100 EtOHaq Conc: 0.100g/210L Range: 0.095 - 0.105 Preparation Date: 5/11/2015 Expires: 5/11/2016 OPENED: Brian Fox 2/7/16	FOX
4/24/16	Officer reports "BLACK error" followed by "FORMIDATA OUT OF RANGE error" on 4/23 [For RPC or Simulator Solution Change Place Label Here] completed: Accuracy + Precision test. Passed w/ 1.096 sim. mpa mure	J. MARCOUX
5/18/16	[For RPC or Simulator Solution Change Place Label Here] DataMaster External Standard Solution Lot # 15-25-100 EtOHaq Conc: 0.100 Range: 0.095 - 0.105 Preparation Date: 11/30/2015 Expires: 11/30/2016 OPENED: 5/18/16 Fox Solution change out of range	Fox
6/18/16	[For RPC or Simulator Solution Change Place Label Here] Officer reports DMT reported as "Busy" in lower left corner; Run was not clear, and nothing happened also run was pushed. I.T. Line nearly added; Run parameters a/o I.T. line in, checks done; plugged I.T. line in - showed "Busy" but after nearly 30 seconds, was able to press run / cancelled AB press run again/cancelled and each time has brought to POC screen w/o issue.	J. Marcoux

DATAMASTER DMT MAINTENANCE LOG

Shelton Police
Department/Agency

100133
DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
6/21/16	DataMaster External Standard Solution [For RPC or Simulator Solution Change Place Label Here] Lot # 15-25-100 EtOHaq Conc: 0.100 Range: 0.095 - 0.105 Preparation Date: 11/30/2015 Expires: 11/30/2016 OPENED: RPC / solution change	B. Fox
10/16/16	DataMaster External Standard Solution [For RPC or Simulator Solution Change Place Label Here] Lot # 16-05-100 EtOHaq Conc: 0.099 Range: 0.094 - 0.104 Preparation Date: 4/19/2016 Expires: 4/19/2017 OPENED: Solution Change / RPC	B. Fox
10/21/16	Completed APM Protocol [For RPC or Simulator Solution Change Place Label Here]	R. Driscoll DMT Tech.
1/20/17	Solution Change [For RPC or Simulator Solution Change Place Label Here] DataMaster External Standard Solution Lot # 16-05-100 EtOHaq Conc: 0.099 Range: 0.094 - 0.104 Preparation Date: 4/19/2016 Expires: 4/19/2017 OPENED:	B. Fox

DATAMASTER DMT MAINTENANCE LOG

Department/Agency

DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
2/23/17	DMT Simulator Solution Lot # 17-07-100 EtOHaq Certified Conc: 0.100 Range: 0.095 - 0.105 Preparation Date: 01/18/2017 Expires: 01/18/2018 OPENED: [For RPC Label Here] RPC / Solution Change	B. Fox
4/2/17	DMT Simulator Solution Lot # 17-07-100 EtOHaq Certified Conc: 0.100 Range: 0.095 - 0.105 Preparation Date: 01/18/2017 Expires: 01/18/2018 OPENED: [For RPC e Label Here] Solution Change	B. Fox
4/7/17	DMT Simulator Solution Lot # 17-16-100 EtOHaq Certified Conc: 0.101 Range: 0.096 - 0.106 Preparation Date: 04/03/2017 Expires: 04/03/2018 OPENED: 4/7/17 DDP [For RP ace Label Here] REINSTALL AFTER HARDWARE UPGRADE	D. PATLAK VFL
6/25/17	[For RPC or Simulator Solution Change Place Label Here] RPC / solution change DMT Simulator Solution Lot # 17-13-100 EtOHaq Certified Conc: 0.101 Range: 0.096 - 0.106 Preparation Date: 02/28/2017 Expires: 02/28/2018 OPENED: 6/25/17 Fox	B. Fox

DATAMASTER DMT MAINTENANCE LOG

Shelburne PD
Department/Agency

100133
DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
10/28/17	<u>RPC & Simulator Chg</u> [For RPC or Simulator Solution Change Place Label Here] DMT Simulator Solution Lot # 17-13-100 EtOHaq Certified Conc: 0.101 Range: 0.096 - 0.106 Preparation Date: 02/28/2017 Expires: 02/28/2018 OPENED: <u>10/23/17</u> <u>Fox</u>	B. Fox
10/31/17	<u>Installed version 2.00 PIC chip</u> [For RPC or Simulator Solution Change Place Label Here]	R. Driscoll VFL
2/22/18	<u>RPC & Solution Chg</u> [For RPC or Simulator Solution Change Place Label Here] DMT Simulator Solution Lot # 17-21-100 EtOHaq Certified Conc: 0.100 Range: 0.095 - 0.105 Preparation Date: 09/20/2017 Expires: 09/20/2018 OPENED: <u>2/22/18</u> <u>Fox</u>	B. Fox
3/7/18	<u>Completed APM Protocol</u> [For RPC or Simulator Solution Change Place Label Here]	R. Driscoll VFL

DATAMASTER DMT MAINTENANCE LOG

Shelburne PD

Department/Agency

160133

DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
6/24	DMT Simulator Solution Lot # 17-21-100 EtOHaq Certified Conc: 0.100 Range: 0.095 - 0.105 Preparation Date: 09/20/2017 Expires: 09/20/2018 OPENED: <u>6/24/18</u> <u>B. Fox</u> [For RPC Label Here] RPC & Soln Change	B. Fox
10/14	DMT External Std Solution Lot: 18-05-100 EtOH Certified Conc. 0.100 Range: 0.095 - 0.105 Prep Date: 3/21/18 Exp Date: 03/21/19 Opened: <u>Fox 10-14-18</u> [For RPC Label Here] RPC & Soln Change	B. Fox
2/26	DMT External Std Solution Lot: 18-19-100 EtOH Certified Conc. 0.101 Range: 0.096 - 0.106 Prep Date: 12/19/18 Exp Date: 12/19/19 Opened: <u>Fox 2-26-19</u> [For RPC or Simulator Solution Change Place Label Here] RPC & Soln Change	B. Fox
3/5/19	Completed ARM protocol [For RPC or Simulator Solution Change Place Label Here]	J Dukette (VFL)

DATAMASTER DMT MAINTENANCE LOG

① Shelby PD
Department/Agency

160133
DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
6/11/19	DMT External Std Solution Lot: 18-19-100 EtOH Certified Conc. 0.101 Range: 0.096 - 0.106 Prep Date: 12/19/18 Exp Date: 12/19/19 Opened: [For F Place Label Here] RPC & solution change B. Fox	B. Fox
9/17/19	troubleshoot ethernet [For RPC or Simulator Solution Change Place Label Here] connection, not online	AS
10/13/19	DMT External Std Solution Lot: 19-07-100 EtOH Certified Conc. 0.103 Range: 0.098 - 0.108 Prep Date: 5/31/19 Exp Date: 05/31/20 Opened: 10/13/19 FOX [For RPC : Label Here] RPC & solution change B. Fox	B. Fox
2/9/20	DMT External Std Solution Lot: 19-07-100 EtOH Certified Conc. 0.103 Range: 0.098 - 0.108 Prep Date: 5/31/19 Exp Date: 05/31/20 Opened: 2-9-20 [For RPC : Label Here] RPC & solution change	B. Fox

DATAMASTER DMT MAINTENANCE LOG

Department/Agency _____

DataMaster DMT Serial Number _____

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
2/25/2020	Completed APM protocol [For RPC or Simulator Solution Change Place Label Here]	J Dukette (VFL)
	DMT supervisor advised there was a problem w/ screen. Adjusted cards and secured connections. Screen works. JSD 2/25/2020	
6/18/20	RPC & Solution Change [For RPC or Simulator Solution Change Place Label Here] DMT External Std Solution Lot: 20-03-100 EtOH Certified Conc. 0.100 Range: 0.095 - 0.105 Prep Date: 1/29/20 Exp Date: 01/29/21 Opened: _____	RUK
7/13/20	Software update [For RPC or Simulator Solution Change Place Label Here]	[Signature]
10/19/20	RPC & Solution Change [For RPC or Simulator Solution Change Place Label Here] DMT External Std Solution Lot: 20-03-100 EtOH Certified Conc. 0.100 Range: 0.095 - 0.105 For 10-19 Prep Date: 1/29/20 Exp Date: 01/29/21 Opened: _____	BKF

DATAMASTER DMT MAINTENANCE LOG

Department/Agency _____

DataMaster DMT Serial Number _____

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
2/4/21	[For RPC or Simulator Solution Change Place Label Here] DMT External Std Solution Lot: 20-14-100 EtOH Certified Conc. 0.100 Range: 0.095 - 0.105 <i>Fox 2/4/21</i> Prep Date: 9/22/20 Exp Date: 09/22/22 Opened: _____ <i>RPC & Solution Change</i>	<i>B. Fox</i>
2/12/2021	<i>Completed APM protocol.</i> [For RPC or Simulator Solution Change Place Label Here] DMT External Std Solution Lot: 20-14-100 EtOH Certified Conc. 0.100 Range: 0.095 - 0.105 Prep Date: 9/22/20 Exp Date: 09/22/22 Opened: _____	<i>S. Stratton (VFL)</i>
6/25/21	[For RPC or Simulator Solution Change Place Label Here] ↓ <i>RPC & solution change</i>	<i>B. Fox</i>
10/23/21	DMT External Std Solution Lot: 21-09-100 EtOH Certified Conc. 0.099 Range: 0.094 - 0.104 <i>nge Place Label Here]</i> Prep Date: 6/4/21 Exp Date: 06/04/23 Opened: _____ <i>RPC & solution change.</i>	<i>B. Miller</i>

DATAMASTER DMT MAINTENANCE LOG

Shelburne

Department/Agency

100133

DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
2/11/22	Completed APM protocol [For RPC or Simulator Solution Change Place Label Here]	J. Dukette (VFL)
2/19/22	DMT External Std Solution [For RPC Lot: 21-09-100 EtOH Certified Conc. 0.099 Range: 0.094 - 0.104 Prep Date: 6/4/21 Exp Date: 06/04/23 Opened: 2/19/22 Miller Place Label Here] RPC	B. Miller M1037
10/21/22	DMT External Std Solution [For RPC Lot: 22-04-100 EtOH Certified Conc. 0.100 Range: 0.095 - 0.105 Prep Date: 1/26/22 Exp Date: 01/26/24 Opened: Place Label Here] RPC Solution Change	D. Eidenburg M1003 SN: 100133
2/3/23	DMT External Std Solution [For RPC Lot: 22-04-100 EtOH Certified Conc. 0.100 Range: 0.095 - 0.105 Prep Date: 1/26/22 Exp Date: 01/26/24 Opened: 2/3/23 MARCOU Place Label Here] RPC	J. MARCOU M1004 S/N 100133

DATAMASTER DMT MAINTENANCE LOG

Department/Agency _____

DataMaster DMT Serial Number _____

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
2/8/23	<i>Completed APM protocol</i> [For RPC or Simulator Solution Change Place Label Here]	S. Stratton (VFL)
6/20/23	DMT External Std Solution Lot: 23-01-100 EtOH Certified Conc. 0.100 [For <i>Fox 6/20/23</i> Place Label Here] Prep Date: 1/25/23 Exp Date: 01/25/25 Opened: <i>RPC & Solution Change</i> <i>Fox</i>	B. Fox
11/27/23	[For RPC or Simulator Solution Change Place Label Here] DMT External Std Solution Lot: 23-07-100 EtOH Certified Conc. 0.100 Prep Date: 6/20/23 Exp Date: 06/20/25 Opened: <i>RPC & Solution Change</i>	B. Fox
2/6/24	<i>Completed APM protocol and removed old operator log</i> [For RPC or Simulator Solution Change Place Label Here]	S. Stratton (VFL)

DATAMASTER DMT MAINTENANCE LOG

Department/Agency _____

DataMaster DMT Serial Number _____

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
2/2/21	<i>RPC & Solution Change</i> [For RPC or Simulator Solution Change Place Label Here] DMT External Std Solution Lot: 23-07-100 EtOH Certified Conc. 0.100 Prep Date: 6/20/23 Exp Date: 06/20/25 Opened: _____	<i>B. Fox</i>
6/23/24	<i>RPC & Solution Change</i> [For RPC or Simulator Solution Change Place Label Here] DMT Quality Control Solution Lot: 24-02-100 EtOH Certified Conc. 0.099 Prep Date: 4/9/24 Exp Date: 04/09/26 Opened: _____	<i>B. Fox</i>
10/8/21	<i>RPC & Solution Change</i> [For RPC or Simulator Solution Change Place Label Here] DMT Quality Control Solution Lot: 24-02-100 EtOH Certified Conc. 0.099 Prep Date: 4/9/24 Exp Date: 04/09/26 Opened: _____	<i>B. Fox</i>
11/21/25	<i>APM</i> [For RPC or Simulator Solution Change Place Label Here]	<i>A. Bolder</i>

DATAMASTER DMT MAINTENANCE LOG

Department/Agency _____

DataMaster DMT Serial Number _____

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
2/27	<i>RPC & Solution Change</i> [For RPC or Simulator Solution Change Place Label Here] DMT Quality Control Solution Lot: 24-17-100 EtOH Certified Conc. 0.100 Prep Date: 10/21/24 <i>BKF</i> Exp Date: 10/21/26 Opened: <i>Failed out of service Filter Wheel</i>	<i>BKF</i>
4/1/25	<i>Removed for Rehub</i> [For RPC or Simulator Solution Change Place Label Here]	<i>SB</i>
	[For RPC or Simulator Solution Change Place Label Here]	
	[For RPC or Simulator Solution Change Place Label Here]	