

DATAMASTER DMT MAINTENANCE LOG

Bradford WSP
Department/Agency

100140
DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
10/27/11	<p>DataMaster Simulator Solution Lot # 12-13-100 EtOH_{aq} Conc: 0.102 Range: 0.097 - 0.107 Preparation Date: 09/09/2011 Expires: 09/09/2012 [For R] Place Label Here]</p> <p>OPENED: 10/27/11 10-27-11</p> <p style="text-align: center;">Install Per Protocol</p>	<p>Steven Harnois</p> <p>10/27/11 10-27-11 Prog. Chief, org. Chem</p>
11/11/11	<p>DataMaster Simulator Solution Lot # 12-13-100 EtOH_{aq} Conc: 0.102 Range: 0.097 - 0.107 Preparation Date: 09/09/2011 Expires: 09/09/2012 [For F] Place Label Here]</p> <p>OPENED: 11/11/11</p> <p>Simulator out of range, changed solution. Changed clock DST.</p>	D. White
12/2/11	<p>DataMaster Simulator Solution Lot # 12-32-100 EtOH_{aq} Conc: 0.100 Range: 0.095 - 0.105 Preparation Date: 10/26/2011 Expires: 10/26/2012 [For] Place Label Here]</p> <p>OPENED: 12/2/11</p> <p>Simulator out of range. Changed solution</p>	D. White
2/11/12	<p>DataMaster Simulator Solution Lot # 12-38-100 EtOH_{aq} Conc: 0.101 Range: 0.096 - 0.106 Preparation Date: 11/17/2011 Expires: 11/17/2012 [For] Place Label Here]</p> <p>OPENED: 2/11/12</p> <p>Simulator out of range / RPC.</p>	D. White

DATAMASTER DMT MAINTENANCE LOG

Bradford VSP

Department/Agency

100140




DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
3/26/12	[For RPC or Simulator Solution Change Place Label Here] Reset Clock DST	DCWR
5/17/12	<u>DataMaster Simulator Solution</u> Lot # 12-58-100 EtOH _{aq} Conc: 0.100 Range: 0.095 - 0.105 Preparation Date: 02/09/2012 Expires: 02/09/2013 [F ge Place Label Here] OPENED: 5/17/12	DCWR
6/27/12	<u>DataMaster Simulator Solution</u> Lot # 12-73-100 EtOH _{aq} Conc: 0.098 Range: 0.093 - 0.103 Preparation Date: 04/27/2012 Expires: 04/27/2013 [ge Place Label Here] OPENED: 6/27/12 DCWR	DCWR
10/19/12	APM Performed [For RPC or Simulator Solution Change Place Label Here]	R. Driscoll

DATAMASTER DMT MAINTENANCE LOG

Bradford VSP
Department/Agency

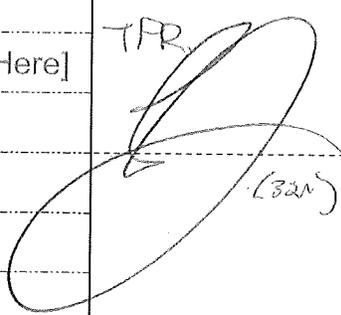
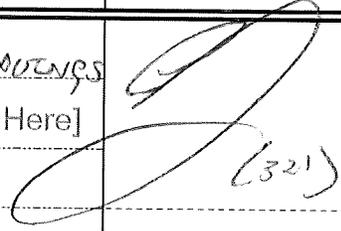
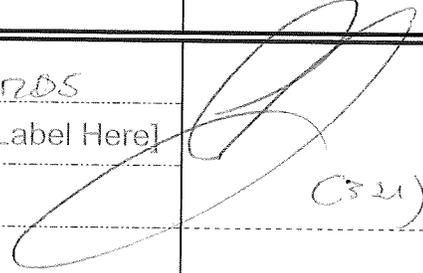

100140
DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
10/30/12	<p>DataMaster Simulator Solution Lot # 12-73-100 EtOHaq Conc: 0.098 Range: 0.093 - 0.103 Preparation Date: 04/27/2012 Expires: 04/27/2013</p> <p>OPENED: 10/30/12</p> <p>TEST /RPC October 2012</p>	DCWB
12.22.12	<p>[For RPC or Simulator Solution Change Place Label Here]</p> <p>PRINTER WOULD NOT PRINT. RESET DMT + PRINTER TO RESTORE FUNCTIONALITY</p>	
12.30.12	<p>Reported For BLANK ERROR ON [For RPC or Simulator Solution Change Place Label Here]</p> <p>12.29.12 DUI PROCESSING. PERFORMED MAINT STEPS PER MANUAL</p>	
1.22.13	<p>[For RPC or Simulator Solution Change Place Label Here]</p> <p>logged in to check DATA ON DUI subject TEST</p>	

DATAMASTER DMT MAINTENANCE LOG

Department/Agency _____

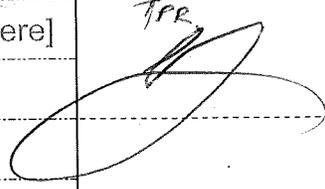
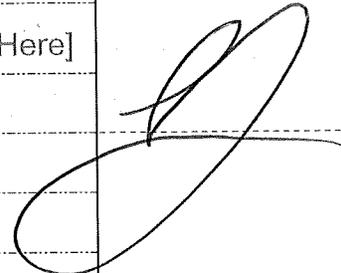
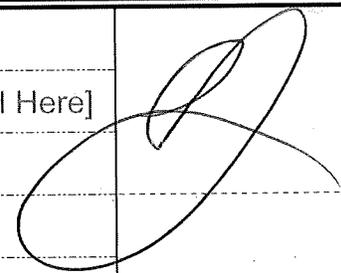
DataMaster DMT Serial Number _____

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
2.3.13	<p style="text-align: center;"><small>OPENED.</small></p> <p>DataMaster Simulator Solution Lot # 12-77-100 EtOHaq Conc: 0.099 Range: 0.094 - 0.104 Preparation Date: 05/08/2012 Expires: 05/08/2013</p> <p style="text-align: center;"><small>CLOSED.</small></p> <p style="text-align: center;">2/13 RPC PASSED</p>	<p style="text-align: center;">TFR</p>  <p style="text-align: right;">(32N)</p>
3.15.13	<p style="text-align: center;">CHANGED TIME FOR DAYLIGHT SAVINGS</p> <p>[For RPC or Simulator Solution Change Place Label Here]</p>	 <p style="text-align: right;">(321)</p>
5.9.13	<p style="text-align: center;">logged on to check records</p> <p>[For RPC or Simulator Solution Change Place Label Here]</p>	 <p style="text-align: right;">(321)</p>
5.22.13	<p style="text-align: center;">logged in to PRINT DMT TICKETS</p> <p>[For RPC or Simulator Solution Change Place Label Here]</p>	 <p style="text-align: right;">321</p>

DATAMASTER DMT MAINTENANCE LOG

Department/Agency _____

DataMaster DMT Serial Number _____

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
6.16.13	<p>[For RPC or Simulator Solution Change Place Label Here]</p> <p>DataMaster Simulator Solution Lot # 12-89-100 EtOHaq Conc: 0.097 Range: 0.092 - 0.102 Preparation Date: 11/21/2012 Expires: 11/21/2013</p> <p>OPENED: 6.16.13</p> <p style="text-align: right;">JUNE RPC</p>	<p>ERIC Jollymore</p> <p>JPR</p> 
8.1.13	<p>[For RPC or Simulator Solution Change Place Label Here]</p> <p>logged on to obtain record history</p>	
8.2.13	<p>UPDATED TIME TO BE IN SYNC WITH [For RPC or Simulator Solution Change Place Label Here]</p> <p>VSP DISPATCH</p>	
10-8-13	<p>[For RPC</p> <p>DataMaster Simulator Solution Lot # 12-88-100 EtOHaq Conc: 0.098 Range: 0.093 - 0.103 Preparation Date: 11/9/2012 Expires: 11/9/2013</p> <p>OPENED: 10/8/13</p> <p style="text-align: right;">October RPC</p>	<p>ice Label Here]</p>  <p>308</p>

DATAMASTER DMT MAINTENANCE LOG

Bradford VSP

Department/Agency

100140

DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
10/17/13	<p style="text-align: center;"><u>Completed AEM Protocol</u></p> <p>[For RPC or Simulator Solution Change Place Label Here]</p>	<p>R. Discol</p> <p>DMT TECH.</p>
12/24/13	<p style="text-align: center;"><u>DataMaster Simulator Solution</u></p> <p>Lot # 13-15-100 EtOHaq Conc: 0.099 Range: 0.094 - 0.104 Preparation Date: 08/9/2013 Expires: 08/9/2014</p> <p>[For _____ Place Label Here]</p> <p>OPENED: 12/24/13 <i>[Signature]</i></p> <p style="text-align: center;">Sim. Sol. change</p>	<p><i>[Signature]</i></p> <p>368</p>
2.5.14	<p>RPC Feb NO EXTRA STICKER</p> <p>[For RPC or Simulator Solution Change Place Label Here]</p> <p style="text-align: center;">Lot 13-19-100 concen: .099</p> <p>prep 10/25/13 EXPIRE</p> <p style="text-align: center;">10/25/14</p>	<p><i>[Signature]</i></p>
5/12/14	<p style="text-align: center;">Sim Sol. change</p> <p>[For RPC or Simulator Solution Change Place Label Here]</p> <p style="text-align: center;">NO EXTRA STICKER</p> <p style="text-align: center;">Lot # 13-19-100 concen. 0.099</p> <p>prep. 10/25/13 - EXO 10/25/14</p> <p style="text-align: center;"><u>DataMaster Simulator Solution</u></p> <p>Lot # 13-19-100 EtOHaq Conc: 0.099 Range: 0.094 - 0.104 Preparation Date: 10/25/2013 Expires: 10/25/2014</p> <p>OPENED: 5/12/14</p>	<p><i>[Signature]</i></p>

DATAMASTER DMT MAINTENANCE LOG

Bradford VSP

Department/Agency

100140

DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
6/27/14	<p>DataMaster Simulator Solution</p> <p>[For RP Lot # 14-04-100 EtOHaq Conc: 0.099 Range: 0.094 - 0.104 Preparation Date: 5/27/2014 Expires: 5/27/2015]</p> <p>OPENED: <u>6/27/14</u></p> <p style="text-align: center;">None RPC</p>	
7/11/14	<p>DataMaster Simulator Solution</p> <p>[For RP Lot # 14-04-100 EtOHaq Conc: 0.099 Range: 0.094 - 0.104 Preparation Date: 5/27/2014 Expires: 5/27/2015]</p> <p>OPENED: <u>7/11/14</u></p> <p style="text-align: center;">Solution Change 7/11/14</p>	
8/18/14	<p>DataMaster Simulator Solution</p> <p>[For Lot # 14-05-100 EtOHaq Conc: 0.098 Range: 0.093 - 0.103 Preparation Date: 6/19/2014 Expires: 6/19/2015]</p> <p>OPENED: <u>8/18/14</u></p> <p style="text-align: center;">Solution Change 8/18/14</p>	
8/19/14	<p>DMT supervisor concerned with sim. solution usage.</p> <p>[For RPC or Simulator Solution Change Place Label Here]</p> <p>Leakchecked simulator and found leak in jar/lid seal. Tightened sim. jar and leak fixed. Also checked all tubing connections. Tower connections seemed loose so cut off ends and snugged tubing.</p>	<p>R. Driscoll DMT Tech.</p>

DATAMASTER DMT MAINTENANCE LOG

Bedford VSP
Department/Agency

100140
DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
10/5/14	<p>DataMaster Simulator Solution [For RPC Lot # 14-10-100 EtOHaq Conc: 0.097 Range: 0.092 - 0.102 Preparation Date: 7/14/2014 Expires: 7/14/2015 OPENED: <u>10/5/14</u> October RPC</p>	
10/24/14	<p>Completed AP4 Protocol [For RPC or Simulator Solution Change Place Label Here]</p>	R. Daseoll DMT TECH.
11/4/14	<p>Changed clock for DST, [For RPC or Simulator Solution Change Place Label Here]</p>	
2/17/15	<p>DataMaster Simulator Solution [For RPC Lot # 14-10-100 EtOHaq Conc: 0.097 Range: 0.092 - 0.102 Preparation Date: 7/14/2014 Expires: 7/14/2015 OPENED: February RPC</p>	

DATAMASTER DMT MAINTENANCE LOG

Bradford USP
Department/Agency

100140
DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
5/28/15	<p>[For RPC or Simulator Solution Change Place Label Here]</p> <p>DataMaster Simulator Solution Lot # 14-14-100 EtOHaq Conc: 0.099 Range: 0.094 - 0.104 Preparation Date: 10/16/2014 Expires: 10/16/2015 OPENED: 5/28/15</p>	Brennan
6/20/15	<p>[For RPC DataMaster Simulator Solution e Label Here]</p> <p>Lot # 14-14-100 EtOHaq Conc: 0.099 Range: 0.094 - 0.104 Preparation Date: 10/16/2014 Expires: 10/16/2015 OPENED: 6/20/15</p>	<p style="text-align: right;">Solution change (out of range)</p> 
8/2/15	<p>[For RPC or Simulator Solution Change Place Label Here]</p> <p>DataMaster Simulator Solution Lot # 15-06-100 EtOHaq Conc: 0.100 g/210L Range: 0.095 - 0.105 Preparation Date: 4/28/2015 Expires: 4/28/2016 OPENED: 8/2/15</p>	<p style="text-align: right;">Solution change out of range</p>
10/11/15	<p>[For RPC DataMaster Simulator Solution e Label Here]</p> <p>Lot # 15-06-100 EtOHaq Conc: 0.100 g/210L Range: 0.095 - 0.105 Preparation Date: 4/28/2015 Expires: 4/28/2016 OPENED: 10/11/15</p> <p style="text-align: center; font-size: 1.2em;">Oct RPC</p>	

DATAMASTER DMT MAINTENANCE LOG

Bradford VSP
Department/Agency

100140
DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
10/29/15	<p>Completed API protocol, Downloaded data to [For RPC or Simulator Solution Change Place Label Here]</p> <p>usb drive, uploaded new software, and installed new I/O PCB. Not connected at this time as Ethernet port is on the opposite side of the room.</p>	R. Driscoll DMT Tech.
11/5/15	<p>DataMaster Simulator Solution Lot # 15-13-100 EtOHaq Conc: 0.099 Range: 0.094 - 0.104 Preparation Date: 09/15/2015 Expires: 09/15/2016</p> <p>[For RPC or _____ _____ label Here]</p> <p>OPENED: <u>11/5/15</u></p> <p>Solution Change</p>	Brennan DMT Sup.
1/26/16	<p>DataMaster External Standard Solution Lot # 15-23-100 EtOHaq Conc: 0.097 Range: 0.092 - 0.102 Preparation Date: 10/29/2015 Expires: 10/29/2016</p> <p>[For RP _____ _____ ice Label Here]</p> <p>OPENED: <u>1/26/16</u></p> <p>Feb RPC</p>	H. Flowers <i>[Signature]</i>
4/2/16	<p>Solution change</p> <p>[For RPC or Simulato</p> <p>DataMaster Simulator Solution Lot # 15-13-100 EtOHaq Conc: 0.099 Range: 0.094 - 0.104 Preparation Date: 09/15/2015 Expires: 09/15/2016</p> <p>OPENED: _____</p>	Brennan

DATAMASTER DMT MAINTENANCE LOG

Bradford VSP
Department/Agency

100140
DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
6/23/16	<div style="border: 1px solid black; padding: 5px; margin-bottom: 10px;"> DataMaster External Standard Solution Lot # 15-23-100 EtOHaq Conc: 0.097 Range: 0.092 - 0.102 Preparation Date: 10/29/2015 Expires: 10/29/2016 OPENED: <u>6/23/16</u> </div> [For RPC] [Place Label Here] RPC	Tps Brennan
10/17/16	<div style="border: 1px solid black; padding: 5px; margin-bottom: 10px;"> DMT External Standard Solution Lot # 16-15-100 EtOHaq Conc: 0.100 Range: 0.095 - 0.105 Preparation Date: 7/20/2016 Expires: 7/20/2017 OPENED: <u>10/17/16</u> </div> [For] [Place Label Here] RPC	Tps Brennan
10/27/16	Completed APM Protocol. [For RPC or Simulator Solution Change Place Label Here] 	R. Driscoll DMT Tech.
1/7/17	<div style="border: 1px solid black; padding: 5px; margin-bottom: 10px;"> DMT External Standard Solution Lot # 16-23-100 EtOHaq Conc: 0.101 Range: 0.096 - 0.106 Preparation Date: 10/19/2016 Expires: 10/19/2017 OPENED: <u>1/7/17</u> </div> [For RPC] [Label Here] Solution Change	Tps Brennan

DATAMASTER DMT MAINTENANCE LOG

Bradford VSP

Department/Agency

100140

DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
	<p>[For RPC DMT External Standard Solution Lot # 16-23-100 EtOHaq Conc: 0.101 Range: 0.096 - 0.106 Preparation Date: 10/19/2016 Expires: 10/19/2017 OPENED: <u>2/15/17 SPB</u> RPC</p>	<p><i>Tps Brennan</i></p>
	<p>[Fo DMT Simulator Solution Lot # 17-10-100 EtOHaq Certified Conc: 0.101 Range: 0.096 - 0.106 Preparation Date: 02/06/2017 Expires: 02/06/2018 OPENED: <u>4/7/17 SPB</u> Solution Change</p>	<p><i>Tps Brennan</i></p>
<p><u>4/13/17</u></p>	<p>[For RF DMT Simulator Solution Lot # 17-16-100 EtOHaq Certified Conc: 0.101 Range: 0.096 - 0.106 Preparation Date: 04/03/2017 Expires: 04/03/2018 OPENED: <u>4/13/17 RD</u> Install post simulator update</p>	<p><i>R. Driscoll VPL</i></p>
<p><u>4/28/17</u></p>	<p>[For F DMT Simulator Solution Lot # 17-10-100 EtOHaq Certified Conc: 0.101 Range: 0.096 - 0.106 Preparation Date: 02/06/2017 Expires: 02/06/2018 OPENED: <u>06/28/17 Haney</u> RPC</p>	<p><i>Tps Haney</i></p>

DATAMASTER DMT MAINTENANCE LOG

Bradford VSP
Department/Agency

100140 100140
DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
10/19/17	<p style="color: blue;">Installed version 2.08 RPC chip and completed APX protocol.</p> <p>[For RPC or Simulator Solution Change Place Label Here]</p>	<p style="color: blue;">R. Driscoll VFL</p>
	<p>DMT Simulator Solution Lot # 17-20-100 EtOHaq Certified Conc: 0.102 Range: 0.097 - 0.107 Preparation Date: 07/07/2017 Expires: 07/07/2018</p> <p>OPENED: 10/28/17 <u>[Signature]</u> SB</p> <p style="font-size: 2em; text-align: center;">RPC</p>	<p><u>[Signature]</u> Tpr Brennan</p>
	<p>DMT Simulator Solution Lot # 17-20-100 EtOHaq Certified Conc: 0.102 Range: 0.097 - 0.107 Preparation Date: 07/07/2017 Expires: 07/07/2018</p> <p>OPENED: 02/18/18 <u>[Signature]</u></p> <p style="font-size: 2em; text-align: center;">RPC</p>	<p><u>[Signature]</u> Tpr Haney</p>
	<p>DMT Simulator Solution Lot # 17-21-100 EtOHaq Certified Conc: 0.100 Range: 0.095 - 0.105 Preparation Date: 09/20/2017 Expires: 09/20/2018</p> <p>OPENED: 06/15/18 <u>[Signature]</u></p> <p style="font-size: 2em; text-align: center;">RPC</p>	<p><u>[Signature]</u> Tpr Haney</p>

DATAMASTER DMT MAINTENANCE LOG

Bradford VSP
Department/Agency

100140
DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
7/18/18	<p style="text-align: center;">Completed RPM Protocol</p> <p>[For RPC or Simulator Solution Change Place Label Here]</p>	R. Driscoll NPL
11/19/18	<p style="text-align: center;">RPC</p> <p style="text-align: center;">DMT External Std Solution</p> <p>[For RPC</p> <p style="text-align: center;">Lot: 18-05-100 EtOH Certified Conc. 0.100</p> <p style="text-align: center;">Range: 0.095 - 0.105</p> <p style="text-align: center;">Prep Date: 3/21/18 Exp Date: 03/21/19</p> <p style="text-align: center;">Opened: 11/19/18 SPB</p> <p style="text-align: right;">ce Label Here]</p>	S. Brennan Trooper
03/04/19	<p style="text-align: center;">RPC</p> <p style="text-align: center;">DMT External Std Solution</p> <p>[For RPC</p> <p style="text-align: center;">Lot: 18-05-100 EtOH Certified Conc. 0.100</p> <p style="text-align: center;">Range: 0.095 - 0.105</p> <p style="text-align: center;">Prep Date: 3/21/18 Exp Date: 03/21/19</p> <p style="text-align: center;">Opened: 3/4/19 SMH</p> <p style="text-align: right;">ce Label Here]</p>	J. Hawley Trooper
6/26/19	<p style="text-align: center;">RPC</p> <p style="text-align: center;">DMT External Std Solution</p> <p>[For RPC</p> <p style="text-align: center;">Lot: 19-01-100 EtOH Certified Conc. 0.101</p> <p style="text-align: center;">Range: 0.096 - 0.106</p> <p style="text-align: center;">Prep Date: 1/15/19 Exp Date: 01/15/20</p> <p style="text-align: center;">Opened: 6/26/19 JMH</p> <p style="text-align: right;">ce Label Here]</p>	J. Hawley Trooper

DATAMASTER DMT MAINTENANCE LOG

Department/Agency _____

DataMaster DMT Serial Number _____

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
7/12/19	<p style="text-align: center;"><i>Completed APM protocol</i></p> <p>[For RPC or Simulator Solution Change Place Label Here]</p>	<i>J Dukette (VFL)</i>
10/30/19	<p style="text-align: center;">DMT External Std Solution</p> <p>Lot: 19-07-100 EtOH Certified Conc. 0.103 Range: 0.098 - 0.108 Prep Date: 5/31/19 Exp Date: 05/31/20 Opened: 10/30/19 <i>SPB</i></p> <p style="text-align: center; font-size: 2em;"><i>RPC</i></p>	<p><i>Sean Brennan</i> Trooper DMT Supervisor</p>
12/22/19	<p style="text-align: center;">DMT External Std Solution</p> <p>Lot: 19-13-100 EtOH Certified Conc. 0.100 Range: 0.095 - 0.105 Prep Date: 9/23/19 Exp Date: 09/23/20 Opened: 12/22/19 <i>SPB</i></p> <p style="text-align: center;"><i>Solution change</i> [change Place Label Here]</p>	<p><i>Sean Brennan</i> Trooper DMT Supervisor</p>
3/7/20	<p style="text-align: center;">DMT External Std Solution</p> <p>Lot: 19-13-100 EtOH Certified Conc. 0.100 Range: 0.095 - 0.105 Prep Date: 9/23/19 Exp Date: 09/23/20 Opened: 3/7/20 <i>SPB</i></p> <p style="text-align: center;"><i>change</i> [Place Label Here]</p>	<p><i>Sean Brennan</i> Trooper DMT Supervisor</p>
7/10/20	<p style="text-align: center;">DMT External Std Solution</p> <p>[For RPC Lot: 20-10-100 EtOH Certified Conc. 0.101 Range: 0.096 - 0.106 Prep Date: 6/25/20 Exp Date: 06/25/22 Opened: <i>5/50 7/10/20</i></p> <p style="text-align: center;"><i>June AP RPC</i> <i>5/50 7/10/20</i></p> <p style="text-align: center;"><i>Completed APM protocol</i></p>	<p><i>J Dukette (VFL)</i></p>

DATAMASTER DMT MAINTENANCE LOG

Department/Agency _____

DataMaster DMT Serial Number _____

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
10-27-20	<p style="text-align: center;">DMT External Std Solution</p> <p>[For RPC] Lot: 20-10-100 EtOH Certified Conc. 0.101</p> <p>Range: 0.096 - 0.106 [Place Label Here]</p> <p>Prep Date: 6/25/20 Exp Date: 06/25/22</p> <p>Opened: 10-27-20 D. Garces</p>	Trooper Garces DMT Supt
11/23/2020	<p>Replaced broken sim - DMT connectors. DMT ready to be returned to service.</p> <p>[For RPC or Simulator Solution Change Place Label Here]</p>	S. Stratton (VFL)
2-25-21	<p style="text-align: center;">DMT External Std Solution</p> <p>[For RPC] Lot: 20-10-100 EtOH Certified Conc. 0.101</p> <p>Range: 0.096 - 0.106 [Place Label Here]</p> <p>Prep Date: 6/25/20 Exp Date: 06/25/22</p> <p>Opened: 2-25-21 D. Garces</p> <p style="text-align: center; font-size: 2em;">RPC</p>	Trooper D. Garces
6/16/21	<p style="text-align: center; font-size: 2em;">RPC</p> <p>[For RPC or Simulator Solution Change Place Label Here]</p> <p style="text-align: center;">DMT External Std Solution</p> <p>Lot: 21-04-100 EtOH Certified Conc. 0.100</p> <p>Range: 0.095 - 0.105</p> <p>Prep Date: 2/12/21 Exp Date: 02/12/23</p> <p>Opened: 6-16-21 D. Garces</p>	Trooper D. Garces

DATAMASTER DMT MAINTENANCE LOG

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
7/2/22	<p style="text-align: center;">DMT External Std Solution</p> <p>[For] Lot: 22-10-100 EtOH Certified Conc. 0.100 Place Label Here]</p> <p>Range: 0.095 - 0.105</p> <p>Prep Date: 4/1/22 Exp Date: 04/01/24</p> <p>Opened:</p> <p style="text-align: center; font-size: 1.5em;">RPC</p>	<p style="font-size: 1.2em;">J. Hauer</p> <p style="font-size: 1.2em;">DMT Sup</p>
10/14/22	<p style="text-align: center; font-size: 1.5em;">RPC</p> <p>[For RF] Lot: 22-12-100 EtOH Certified Conc. 0.101 Place Label Here]</p> <p>Range: 0.096 - 0.106</p> <p>Prep Date: 5/31/22 Exp Date: 05/31/24</p> <p>Opened: 10-14-22 D. Garces</p> <p style="text-align: center; font-size: 1.5em;">RPC</p>	<p style="font-size: 1.2em;">D. Garces</p>
3/31/23	<p style="text-align: center; font-size: 1.5em;">RPC</p> <p>[For RPC or Simulator Solution Change Place Label Here]</p> <p style="text-align: center;">DMT External Std Solution</p> <p>Lot: 23-02-100 EtOH Certified Conc. 0.101</p> <p>Prep Date: 2/24/23 Exp Date: 02/24/25</p> <p>Opened: 3-31-23 D. Garces</p>	<p style="font-size: 1.2em;">D. Garces</p>
6/18/23	<p style="text-align: center; font-size: 1.5em;">RPC</p> <p>[For RPC or Simulator Solution Change Place Label Here]</p> <p style="text-align: center;">DMT External Std Solution</p> <p>Lot: 23-02-100 EtOH Certified Conc. 0.101</p> <p>Prep Date: 2/24/23 Exp Date: 02/24/25</p> <p>Opened: D. Garces 6-18-23</p>	<p style="font-size: 1.2em;">D. Garces</p>

DATAMASTER DMT MAINTENANCE LOG

Department/Agency _____

DataMaster DMT Serial Number _____

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
6/27/23	<p style="text-align: center; font-size: 1.2em; color: blue;">Completed APM</p> <p>[For RPC or Simulator Solution Change Place Label Here]</p>	<p style="font-size: 1.2em; color: blue;">J Dulcote (VFC)</p>
11-04-23	<p style="text-align: center; font-size: 1.5em;">RPC</p> <p>[For RPC or Simulator Solution Change Place Label Here]</p> <div style="border: 1px solid black; padding: 5px; margin: 5px 0;"> <p style="text-align: center; margin: 0;">DMT External Std Solution</p> <p style="margin: 0;">Lot: 23-06-100 EtOH Certified Conc. 0.100</p> <p style="margin: 0;">Prep Date: 5/1/23 Exp Date: 05/01/25</p> <p style="margin: 0;">Opened: 11-04-23 D. Garces</p> </div>	<p style="font-size: 1.2em;">D. Garces</p>
02/29/24	<p style="text-align: center; font-size: 1.2em;">DMT External Std Solution</p> <p>[For Lot: 23-10-100 EtOH Certified Conc. 0.099 Place Label Here]</p> <p style="margin-left: 20px;">Prep Date: 11/28/23 Exp Date: 11/28/25</p> <p style="margin-left: 20px;">Opened: _____</p> <p style="text-align: center; font-size: 1.5em; margin-top: 10px;">RPC</p>	<p style="font-size: 1.2em;">J. Hacey</p>
02/01/24	<p style="text-align: center; font-size: 1.2em;">DMT External Std Solution</p> <p>[For R Lot: 23-10-100 EtOH Certified Conc. 0.099 Place Label Here]</p> <p style="margin-left: 20px;">Prep Date: 11/28/23 Exp Date: 11/28/25</p> <p style="margin-left: 20px;">Opened: Hacey 01/01/24</p> <p style="text-align: center; font-size: 1.5em; margin-top: 10px;">RPC</p>	<p style="font-size: 1.2em;">J. Hacey</p>

DATAMASTER DMT MAINTENANCE LOG

Department/Agency _____

DataMaster DMT Serial Number _____

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
6/25/24	<p style="font-size: 1.2em; color: blue;">Completed ARM</p> <p>[For RPC or Simulator Solution Change Place Label Here]</p>	J Dukett (VFC)
10/23/24	<p style="text-align: center;">DMT External Std Solution</p> <p>Lot: 23-10-100 EtOH Certified Conc. 0.099</p> <p>[For RF _____ ace Label Here]</p> <p>Prep Date: 11/28/23 Exp Date: 11/28/25</p> <p>Opened: JMM</p>	JMM
02/17/25	<p style="text-align: center;">DMT Quality Control Solution</p> <p>Lot: 24-07-100 EtOH Certified Conc. 0.100</p> <p>_____ ange Place Label Here]</p> <p>Prep Date: 5/29/24 Exp Date: 05/29/26</p> <p>Opened: 2/17/25 JMM</p>	Haley
4/6/25	<p style="text-align: center;">DMT Quality Control Solution</p> <p>RPC Lot: 25-11-100 EtOH Certified Conc. 0.102</p> <p>_____</p> <p>Prep Date: 4/7/25 Exp Date: 04/07/27</p> <p>Opened: 6/6/25 Haley</p>	Haley
6/19/25	<p style="font-size: 1.2em;">Removed for refurb</p> <p>[For RPC or Simulator Solution Change Place Label Here]</p>	J Dukett (VFC)