


INSTALLATION REPORT

DataMaster DMT: 100140
Location: Bradford VSP
Calibration Date: 10/20/2011
Certification Date: 10/20/2011
Installation Date: 10/27/2011
Installed by: STEVEN E HARNOIS

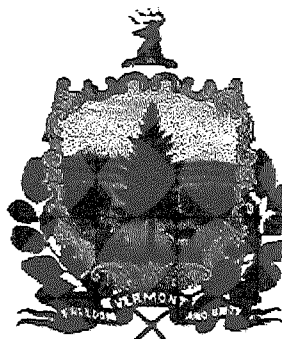

Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

VERSIONS
DMT: 1.00
PIC: 2.05
Modem: 2.1
Questions: 2.0

TEMPERATURES

Sample Chamber = 48.9°C
Breath Tube = 47.1°C
Digital Sim = 33.9°C

SETTINGS

Lamp Voltage = 1.54 V
Cooler Voltage = 1.50 V
Bias Voltage = 80 V
Chopper Freq = 530 Hz

PUMP INFO

Flow Rate = 5.350 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.0827	0.0856
MIN (V)	0.0797	0.0837

FILTER INFO

Filter	Value	Zero
Filter 1	0.085	true
Filter 2	0.464	true
Filter 3	1.002	true

CALIBRATION CHECK

Xq = 0.077 0.45%

Accuracy and Precision Check


Concentration	= 0.102 g/210L
Lot #	= 12-13-100
Range	= 0.097 - 0.107
Average	= 0.100 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

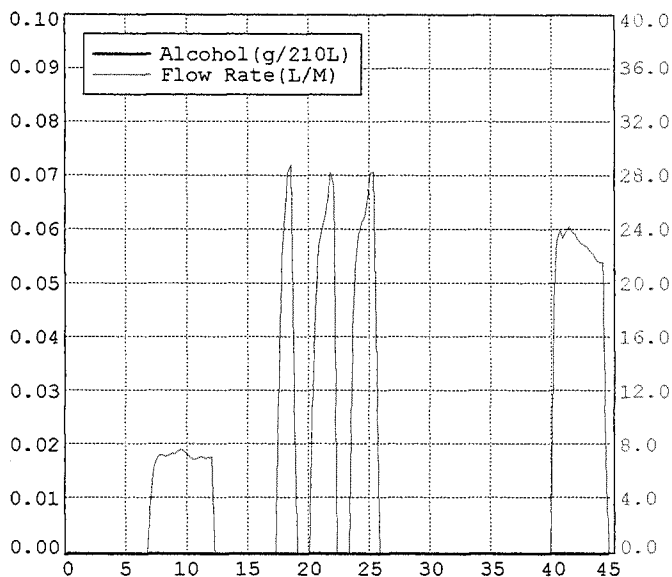

INSTALLATION PASSED

Reviewed 10/28/11
SEB

Performed by *SEB*

Date 10/27/2011

Reviewed by *SEB*

Date 10-27-11