

ROUTINE PERFORMANCE CHECK REPORT



DataMaster DMT: 100140
Location: Bradford VSP
Calibration Date: 10/20/2011
Certification Date: 10/20/2011
Installation Date: 10/27/2011
RPC Date: 10/30/2012
Supervisor Name: DAVID C WHITE

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube = 48.1°C
Digital Sim = 34.2°C

SETTINGS

Lamp Voltage = 1.54 V
Cooler Voltage = 1.51 V
Bias Voltage = 80 V
Chopper Freq = 543 Hz

PUMP INFO

Flow Rate = 5.515 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.1994	0.2022
MIN (V)	0.1982	0.2008

FILTER INFO

Filter 1	0.201	Zero = true
Filter 2	0.572	Zero = true
Filter 3	1.142	Zero = true

CALIBRATION CHECK

Xq = 0.077 0.56%

Routine Performance Check Passed

Accuracy and Precision Check


Concentration	= 0.098 g/210L
Lot #	= 12-73-100
Range	= 0.093 - 0.103
Average	= 0.100 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

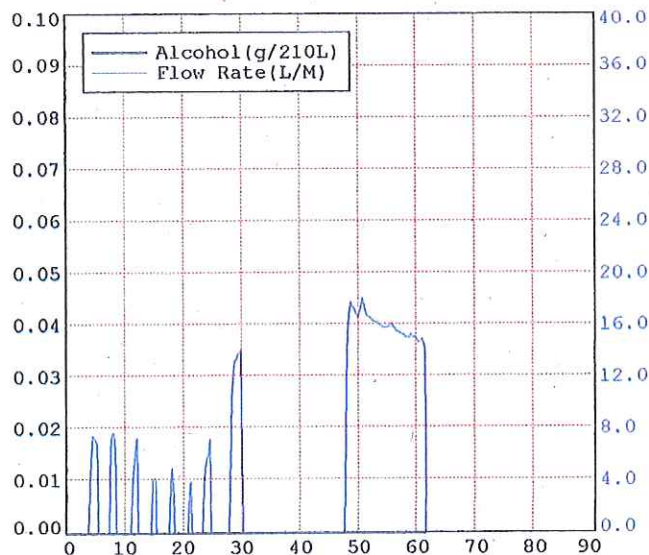

Performed by

[Signature]

Date

10/30/2012

Reviewed by

[Signature]

Date

10/31/12

DMT Serial Number #100140

Page 1 of 1

10/30/2012 2:08 PM

[Signature]
10/31/2012