

ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 100140
Location: Bradford VSP
Calibration Date: 10/20/2011
Certification Date: 10/20/2011
Installation Date: 10/27/2011
RPC Date: 10/05/2014
Supervisor Name: HEATHER A FLOWERS



Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.2°C
Breath Tube = 41.5°C
Digital Sim = 34.1°C

SETTINGS

Lamp Voltage = 1.54 V
Cooler Voltage = 1.50 V
Bias Voltage = 80 V
Chopper Freq = 540 Hz

PUMP INFO

Flow Rate = 5.361 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.3317	0.3352
MIN (V)	0.3305	0.3344

FILTER INFO

Filter 1	0.334	Zero = true
Filter 2	0.697	Zero = true
Filter 3	1.213	Zero = true

CALIBRATION CHECK

Xq = 0.077 0.45%

Accuracy and Precision Check


Concentration	= 0.097 g/210L
Lot #	= 14-10-100
Range	= 0.092 - 0.102
Average	= 0.097 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

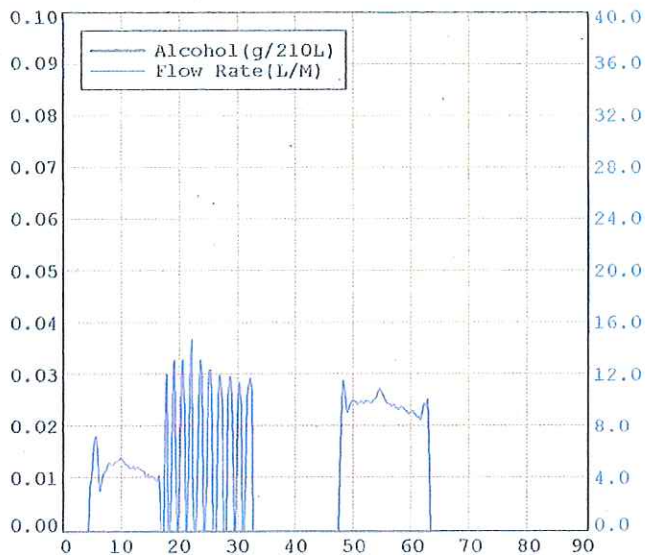

Routine Performance Check Passed

Performed by

Date

10/05/2014

Reviewed by

Date

10/6/14

DMT Serial Number #100140

Page 1 of 1

10/05/2014 10:46 PM

10/6/2014