

INSTALLATION REPORT

DataMaster DMT: 100144
Location: Springfield PD
Calibration Date: 07/02/2012
Certification Date: 07/02/2012
Installation Date: 07/03/2012
Installed by: TRISHA L CONTI



Default Options Loaded

Diagnostic Results

VERSIONS

DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.1°C
Breath Tube = 48.1°C
Digital Sim = 34.2°C

SETTINGS

Lamp Voltage = 1.63 V
Cooler Voltage = 1.61 V
Bias Voltage = 80 V
Chopper Freq = 528 Hz

PUMP INFO

Flow Rate = 5.311 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.0539	0.0581
MIN (V)	0.0522	0.0563

FILTER INFO

Filter	Value	Zero
Filter 1	0.057	true
Filter 2	0.694	true
Filter 3	1.567	true

CALIBRATION CHECK

Xq = 0.080 0.00%

Accuracy and Precision Check


Concentration	= 0.100 g/210L
Lot #	= 12-45-100
Range	= 0.095 - 0.105
Average	= 0.103 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

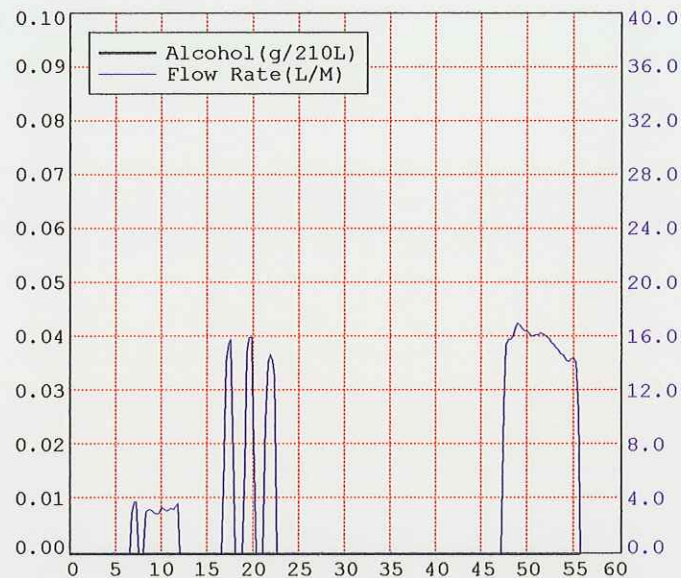

INSTALLATION PASSED

Performed by

TLCA

Date

07/03/2012

Reviewed by

ABolch

Date

7/3/12

TLCA
7/5/2012