

ROUTINE PERFORMANCE CHECK REPORT



DataMaster DMT: 100144
Location: Springfield PD
Calibration Date: 07/02/2012
Certification Date: 07/02/2012
Installation Date: 07/03/2012
RPC Date: 10/18/2015
Supervisor Name: GREGORY J MOLGANO

Diagnostic Results

VERSIONS

DMT: 2.00
PIC: 2.05
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.6°C
Breath Tube = 48.1°C
Digital Sim = 34.1°C

SETTINGS

Lamp Voltage = 1.63 V
Cooler Voltage = 1.61 V
Bias Voltage = 80 V
Chopper Freq = 538 Hz

PUMP INFO

Flow Rate = 5.534 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	0.2596	0.2620
MIN(V)	0.2581	0.2602

FILTER INFO

Filter	Value	Zero
Filter 1	0.261	true
Filter 2	0.865	true
Filter 3	1.722	true

CALIBRATION CHECK

Xq = 0.080 0.65%

Routine Performance Check Passed

Accuracy and Precision Check


Concentration = 0.099 g/210L
Lot # = 15-13-100
Range = 0.094 - 0.104
Average = 0.103 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

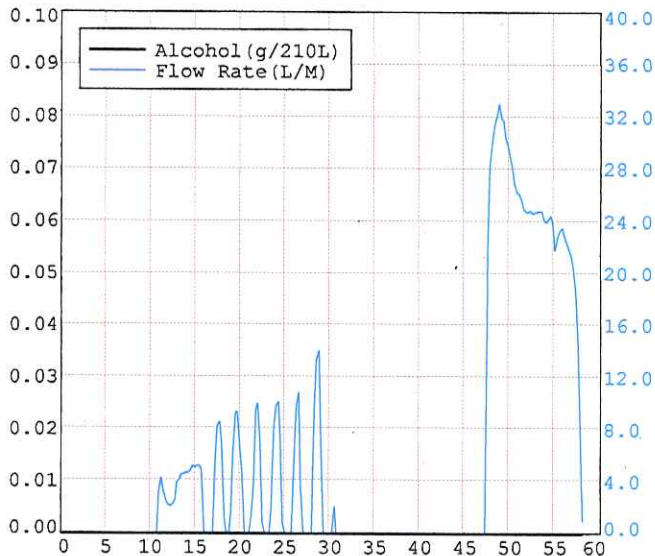

Performed by

Gregory J Molgano

Date

10/18/2015

Reviewed by

[Signature]

Date

10/19/15

DMT Serial Number #100144

Page 1 of 1

10/18/2015 11:57 PM