

INSTALLATION REPORT

DataMaster DMT: 100144
Location: SPRINGFIELD PD
Calibration Date: 04/14/2017
Certification Date: 04/14/2017
Installation Date: 04/18/2017
Installed by: ROBERT DRISCOLL



Default Options Loaded

Diagnostic Results

VERSIONS
DMT: 2.03
PIC: 2.05
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.1°C
Breath Tube = 45.7°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.66 V
Cooler Voltage = 1.66 V
Bias Voltage = 80 V
Chopper Freq = 536 Hz

PUMP INFO

Flow Rate = 5.548 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.0821	0.0852
MIN (V)	0.0809	0.0837

FILTER INFO

Filter 1	0.084	Zero = true
Filter 2	0.709	Zero = true
Filter 3	1.599	Zero = true

CALIBRATION CHECK

Xq = 0.081 0.53%

INSTALLATION PASSED

Accuracy and Precision Check


Concentration	= 0.101 g/210L
Lot #	= 17-16-100
Range	= 0.096 - 0.106
Average	= 0.100 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

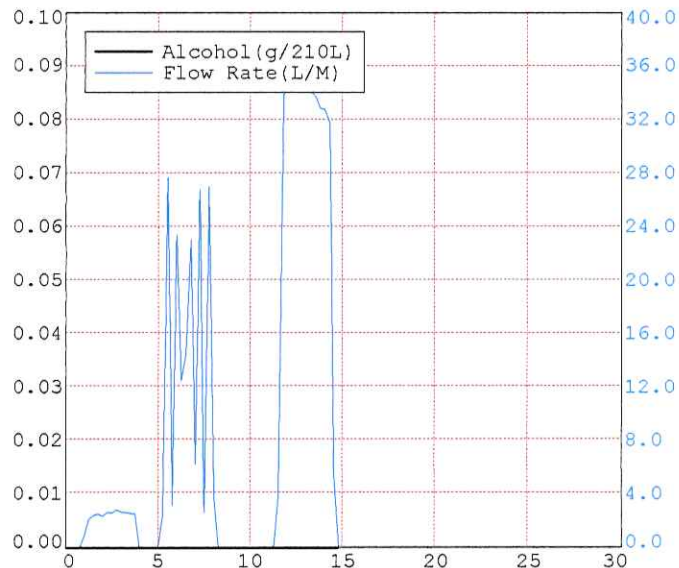

Performed by

RD

Date

04/18/2017

Reviewed by

Date

4/20/17