

INSTALLATION REPORT

DataMaster DMT: 100145
Location: BRIGHTON PD
Calibration Date: 04/27/2017
Certification Date: 04/27/2017
Installation Date: 04/28/2017
Installed by: ROBERT DRISCOLL



Default Options Loaded

Diagnostic Results

VERSIONS
DMT: 2.03
PIC: 2.05
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.9°C
Breath Tube = 48.0°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.63 V
Cooler Voltage = 1.60 V
Bias Voltage = 80 V
Chopper Freq = 533 Hz

PUMP INFO

Flow Rate = 5.607 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	0.0693	0.0744
MIN(V)	0.0677	0.0717

FILTER INFO

Filter	Value	Zero
Filter 1	0.073	true
Filter 2	0.658	true
Filter 3	1.512	true

CALIBRATION CHECK

Xq = 0.125 0.28%

INSTALLATION PASSED

Accuracy and Precision Check


Concentration	= 0.101 g/210L
Lot #	= 17-16-100
Range	= 0.096 - 0.106
Average	= 0.100 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

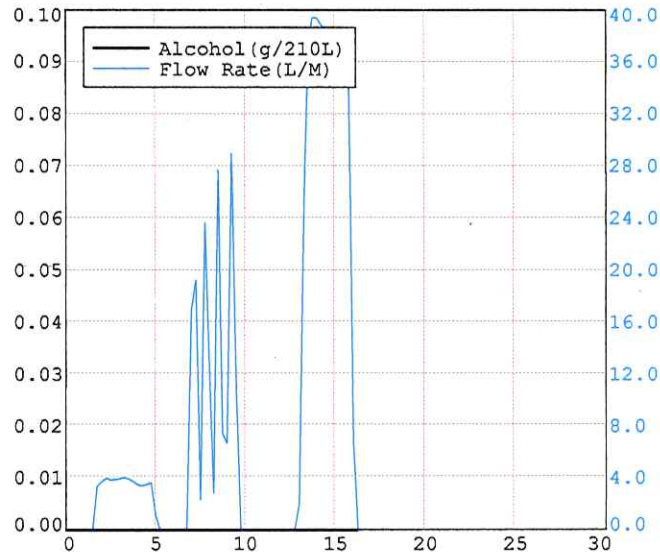

Performed by

RD

Date

04/28/2017

Reviewed by

[Signature]

Date

5/1/17