

ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 100145
Location: BRIGHTON PD
Calibration Date: 04/27/2017
Certification Date: 04/27/2017
Installation Date: 04/28/2017
RPC Date: 11/17/2017
Supervisor Name: JEFFERY M NOYES



Diagnostic Results

VERSIONS
DMT: 2.03
PIC: 2.08
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube = 45.6°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.63 V
Cooler Voltage = 1.60 V
Bias Voltage = 80 V
Chopper Freq = 539 Hz

PUMP INFO

Flow Rate = 5.683 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.1258	0.1313
MIN (V)	0.1244	0.1293

FILTER INFO

Filter	Value	Zero
Filter 1	0.130	true
Filter 2	0.704	true
Filter 3	1.552	true

CALIBRATION CHECK

Xq = 0.124 0.64%

Routine Performance Check Passed

Accuracy and Precision Check


Concentration = 0.100 g/210L
Lot # = 17-21-100
Range = 0.095 - 0.105
Average = 0.100 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

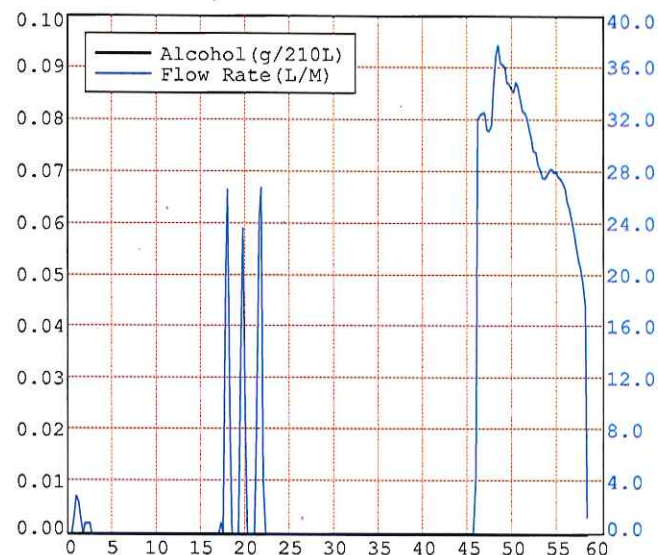

Performed by

Jeffery M. Noyes

Date

11/17/2017

Reviewed by

[Signature]

Date

1/19/18

DMT Serial Number #100145

Page 1 of 1

11/17/2017 9:42 AM