



State of Vermont
Department of Public Safety
VERMONT FORENSIC LABORATORY
45 State Dr. Waterbury, VT 05671

t: 802-244-8788
f: 802-241-5557
DPS.DMT@vermont.gov
<http://vfl.vermont.gov>

Certification of Calibration

Intox DMT Serial # 100145

Date of Adjustment: 01/21/25

Date of Calibration: 01/22/26

Calibration Results:

Instrument was adjusted and calibrated in accordance with Vermont Forensic Laboratory procedure TOX_P200_DMT Manual. The calibration of this instrument is valid for 12 months from the date of calibration. Calibration results are reported as $X \pm Y$, where X is the measured value, Y is the measurement uncertainty.

As Found/As Left

Measured Value	Uncertainty
0.017 $\pm$	0.001 g/210 L
0.080 $\pm$	0.003 g/210 L
0.098 $\pm$	0.004 g/210 L
0.156 $\pm$	0.006 g/210 L
0.356 $\pm$	0.014 g/210 L

The measurement uncertainty for determining the ethanol concentration of aqueous solutions during the in-house calibration of the DMT evidential breath testing instrument is:

3.8%

$k = 2.003$

Uncertainty is expressed as an expanded uncertainty at a 95.45% level of confidence and a coverage factor (k) denoted above, in accordance with ISO/IEC 17025 and ANAB Accreditation Requirements for Forensic Testing and Calibration. The uncertainty associated with this analytical method has been calculated to incorporate uncertainty from the NIST traceable certified reference materials used to adjust and calibrate the instrument, simulator temperature calibration, simulator performance, and analytical performance of the instrument. The uncertainty estimate was evaluated using the VFL fleet of DMT instruments deployed in the field, including the DMT certified in this report.

Traceability to SI through NIST

This calibration is traceable to the International System of Units (SI) through the National Institute of Standards and Technology (NIST) via an unbroken chain of comparisons. The DMT instrument was calibrated using certified reference materials (CRMs). The performance of the calibration was evaluated using NIST traceable control material from an ISO 17034 accredited supplier.

Analyzed CRM materials were prepared using pipettes calibrated by an ISO 17025 accredited calibration vendor. The instrument used to analyze the CRMs was calibrated using NIST traceable certified reference materials from an ISO 17034 accredited supplier. The performance of the method was evaluated using NIST traceable control materials from an ISO 17034 accredited supplier.

Calibration Certified by: *Brittany*
Title: Forensic Chemist
Date: January 23, 2026

This document pertains only to the instrument being calibrated and shall not be reproduced, except in full, without written permission of the Vermont Forensic Laboratory.



State of Vermont
Department of Public Safety
VERMONT FORENSIC LABORATORY
45 State Drive Waterbury, VT 05671

t: 802-244-8788
f: 802-241-5557
DPS.DMT@vermont.gov
<http://vfl.vermont.gov>

DMT Technical Support Inquiry

DMT Serial #: 100145
Date Initiated: 1/20/2026
Initiated By: BMS

Problem:

DMT was removed for annual calibration.

Work Performed:

Upon arrival to the lab for maintenance, it was observed that the tubing to the exhaust port was missing. The tubing was replaced, and the DMT was calibrated. DMT is now ready for installation in the field.

Performed On-Site ☐
Performed In-House ☒

Performed By:	<u>Brittany Shumway <i>Brittany Shumway</i></u>	Date:	<u>1/23/2026</u>
Technical Reviewer:	<u><i>[Signature]</i></u>	Date:	<u>1/29/26</u>
Administrative Reviewer:	<u><i>[Signature]</i></u>	Date:	<u>2/5/26</u>
Director Reviewer:	<u><i>[Signature]</i></u>	Date:	<u>2/6/2026</u>

CALIBRATION REPORT

DataMaster DMT: 100145
Adjustment Date: 1/21/2025
Calibration Date: 1/22/2026
Calibrated by: BRITTANY SHUMWAY



Diagnostic Results

VERSIONS

DMT: 2.07
PIC: 2.08
Modem: 3.0
Questions: 3.0

TEMPERATURES

Sample Chamber = 49.4°C
Breath Tube = 47.8°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.86 V
Cooler Voltage = 1.67 V
Bias Voltage = 80 V
Chopper Freq = 514 Hz

PUMP INFO

Flow Rate = 5.846 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	-0.1142	-0.1098
MIN(V)	-0.1161	-0.1122

FILTER INFO

Filter 1	-0.111	Zero = true
Filter 2	-0.085	Zero = true
Filter 3	0.811	Zero = true

Options

OPTIONS

Units

Alcohol..... g/210L

Simulator

Tolerance Check..... yes
Standard Type..... wet
Nominal..... 0.100
Digital Simulator..... Guth

Subject

Ask Questions..... yes
Number of Tests..... 2
Alcohol Display..... yes
Volume Display..... yes
Query Refusal..... yes
Copies..... 3
Simulator Before..... yes
Simulator Between..... yes
Simulator After..... no
Observation Time..... 0

Supervisor

Number of Tests..... 10

Adjustment

Standard Type..... wet
Nominal..... 0.100
Nominal(Dry Gas)..... 0.100
Number of Tests..... 1

Printer

Printer On..... yes

Software Configuration

Data Collection..... yes

Linearity Check Results

True Value	Reported Average	Std Dev
0.020 g/210L	0.017 g/210L	0.0002
Lot # 25-07-020		
0.081 g/210L	0.080 g/210L	0.0003
Lot # 25-16-080		
0.162 g/210L	0.156 g/210L	0.0004
Lot # 25-05-160		
0.366 g/210L	0.356 g/210L	0.0005
Lot # 25-22-360		

$R^2 = 0.9999$

Acetone Interference Test

Lot # 25-23-08A01

Interference Detected

Mouth Alcohol Test

Mouth Alcohol Detected



RF Detection Test

Passed

Sample Acceptance Test

Passed

CALIBRATION PASSED

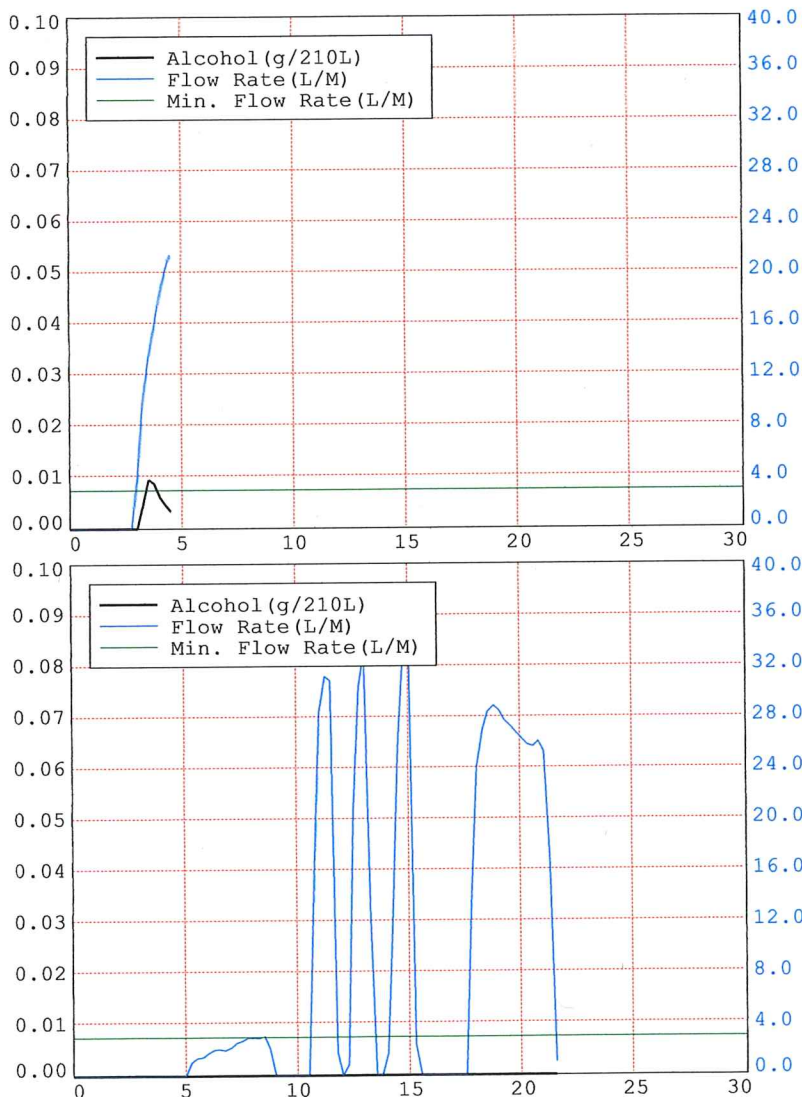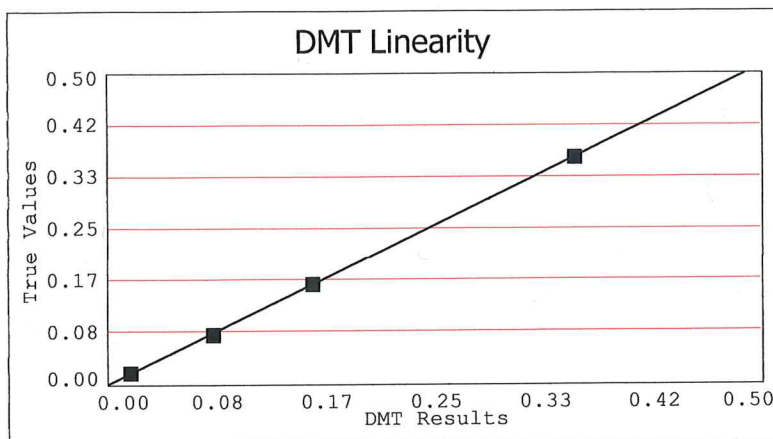

Performed by

Brutney Long

Date

1/22/2026

Reviewed by

[Signature]

Date

1/29/2026

DMT Serial Number #100145

Page 2 of 2

1/22/2026 1:58 PM

100145

BMS

3



ACCURACY & PRECISION REPORT

STATE OF VERMONT

DataMaster DMT: 100145

Date: 1/22/2026

Time: 14:00:28

SUPERVISOR NAME:

BMS MCS

SOLUTION LOT #: 24GP41260

SOLUTION CONCENTRATION: 0.100


BLANK TEST	0.000	14:01
SIMULATOR VAPOR 34.0°C	0.094	14:01
X[1] = 0.0935 (-0.0010) (0.0011)		
SIMULATOR VAPOR 34.0°C	0.094	14:02
X[1] = 0.0942 (-0.0002) (0.0015)		
SIMULATOR VAPOR 34.0°C	0.094	14:04
X[1] = 0.0944 (-0.0009) (0.0013)		
SIMULATOR VAPOR 34.0°C	0.094	14:05
X[1] = 0.0943 (-0.0016) (0.0012)		
SIMULATOR VAPOR 34.0°C	0.094	14:06
X[1] = 0.0943 (-0.0007) (0.0016)		
SIMULATOR VAPOR 34.0°C	0.094	14:07
X[1] = 0.0944 (-0.0004) (0.0017)		
SIMULATOR VAPOR 34.0°C	0.094	14:08
X[1] = 0.0941 (-0.0008) (0.0010)		
SIMULATOR VAPOR 34.0°C	0.094	14:09
X[1] = 0.0937 (-0.0015) (0.0009)		
SIMULATOR VAPOR 34.0°C	0.094	14:11
X[1] = 0.0941 (-0.0006) (0.0012)		
SIMULATOR VAPOR 34.0°C	0.094	14:12
X[1] = 0.0942 (-0.0013) (0.0015)		
BLANK TEST	0.000	14:13

Average = 0.094

Std Dev = 0.0003

* New solution run

BMS 1/22/26

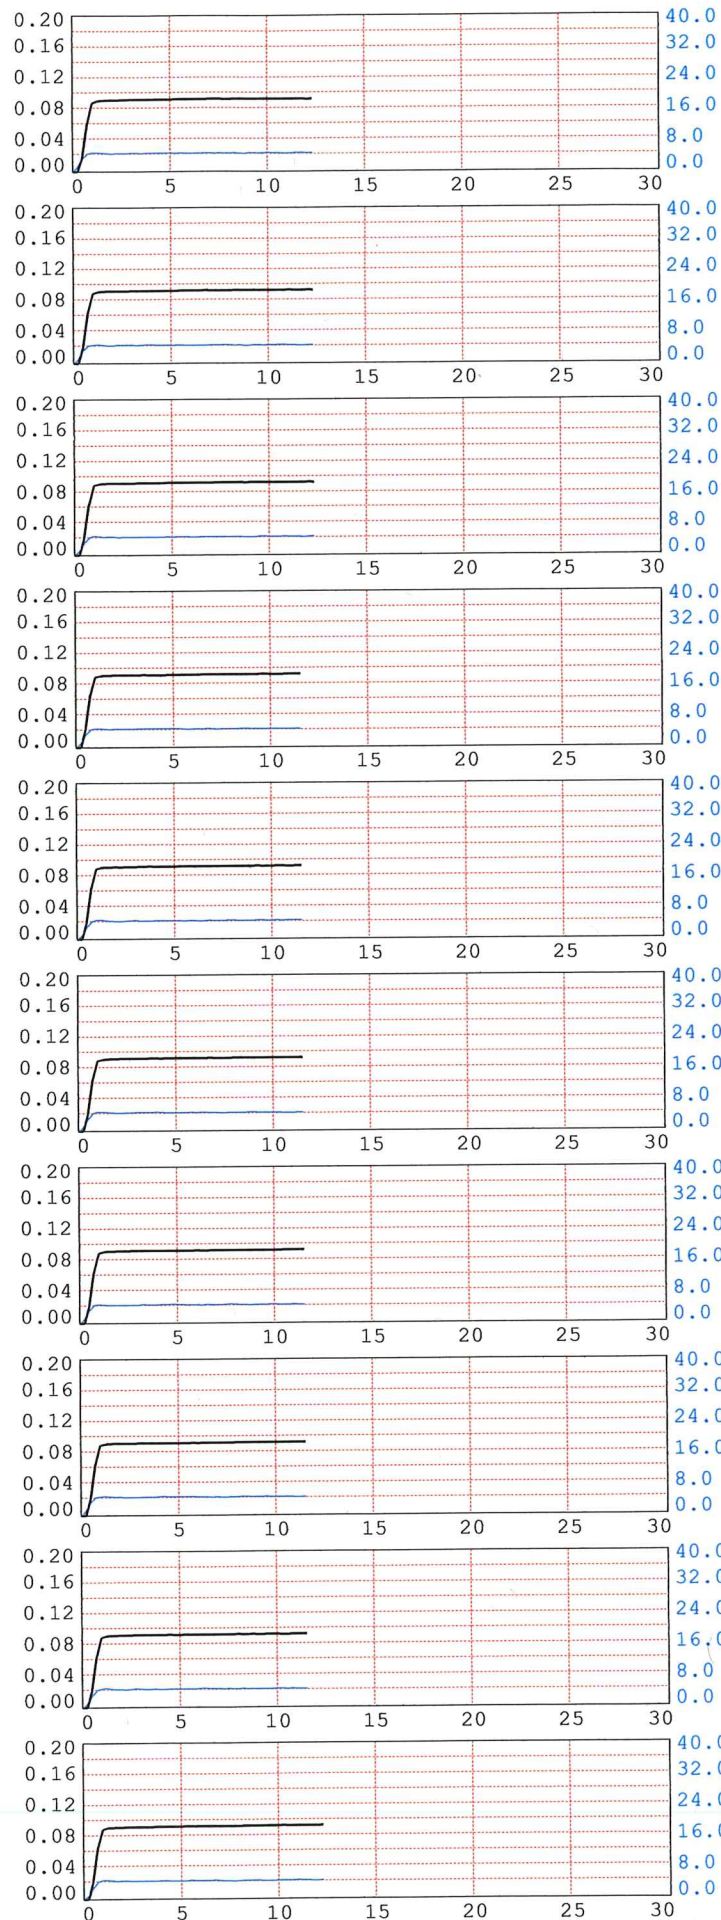



ACCURACY & PRECISION REPORT

STATE OF VERMONT

DataMaster DMT: 100145

Date: 1/22/2026

Time: 14:55:27

SUPERVISOR NAME:

BMS MCS

SOLUTION LOT #: 24GP41260

SOLUTION CONCENTRATION: 0.100

BLANK TEST	0.000	14:56
SIMULATOR VAPOR 34.0°C	0.098	14:56
X[1] = 0.0980 (-0.0001) (0.0019)		
SIMULATOR VAPOR 34.0°C	0.098	14:57
X[1] = 0.0983 (-0.0003) (0.0006)		
SIMULATOR VAPOR 34.0°C	0.099	14:59
X[1] = 0.0987 (-0.0017) (0.0005)		
SIMULATOR VAPOR 34.0°C	0.099	15:00
X[1] = 0.0988 (-0.0009) (0.0009)		
SIMULATOR VAPOR 34.0°C	0.099	15:01
X[1] = 0.0990 (-0.0003) (0.0009)		
SIMULATOR VAPOR 34.0°C	0.098	15:02
X[1] = 0.0981 (-0.0010) (0.0007)		
SIMULATOR VAPOR 34.0°C	0.098	15:04
X[1] = 0.0982 (-0.0015) (0.0011)		
SIMULATOR VAPOR 34.0°C	0.098	15:05
X[1] = 0.0980 (-0.0010) (0.0012)		
SIMULATOR VAPOR 34.0°C	0.098	15:06
X[1] = 0.0981 (-0.0012) (0.0013)		
SIMULATOR VAPOR 34.0°C	0.098	15:07
X[1] = 0.0980 (-0.0016) (0.0014)		
BLANK TEST	0.000	15:08

Average = 0.098

Std Dev = 0.0004

