

INSTALLATION REPORT

DataMaster DMT: 100146
Location: Middlesex VSP
Calibration Date: 11/03/2011
Certification Date: 11/03/2011
Installation Date: 12/06/2011
Installed by: STEVEN E HARNOIS



Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.2
Questions: 2.0

TEMPERATURES

Sample Chamber = 49.1°C
Breath Tube = 47.6°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.69 V
Cooler Voltage = 1.59 V
Bias Voltage = 80 V
Chopper Freq = 546 Hz

PUMP INFO

Flow Rate = 5.985 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.0331	0.0364
MIN (V)	0.0315	0.0350

FILTER INFO

Filter	Value	Zero
Filter 1	0.035	true
Filter 2	0.272	true
Filter 3	0.550	true

CALIBRATION CHECK

Xq = 0.076 0.34%

Accuracy and Precision Check


Concentration	= 0.101 g/210L
Lot #	= 12-38-100
Range	= 0.096 - 0.106
Average	= 0.101 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

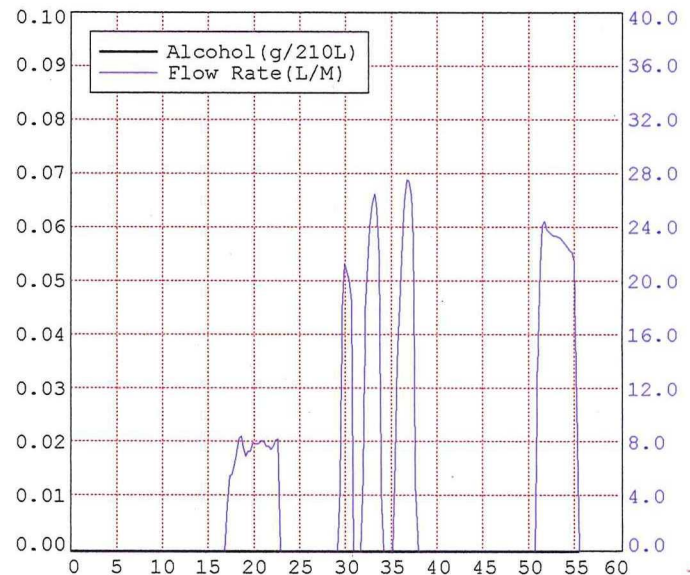

INSTALLATION PASSED

Performed by

Date 12/06/2011

Reviewed by

Date 12/06/11

DMT Serial Number #100146

Page 1 of 1

12/06/2011 1:59 PM

Rev.
12-6-11