

DMT Verification Summary

DMT Serial Number: 100146

	Date	Initial	Solution Lot #	Target	Result	St. Dev.	Bias	% CV	Notes
Adjustment	9/8/2025	ALB	25-13-100	Cal Factor:	0.974022				
Calibration	9/10/2025	ALB							
MCS Check	9/10/2025	ALB	24GP41260	0.100	0.100	0.0006	0.00%	0.60%	
Linearity #1	9/11/2025	ALB	24-22-025	0.025	0.024	0.0002	-4.00%	0.83%	
			25-14-200	0.207	0.197	0.0003	-4.83%	0.15%	
			24-19-340	0.347	0.332	0.0002	-4.32%	0.06%	
Linearity #2	9/12/2025	ALB	24-22-025	0.025	0.024	0.0004	-4.00%	1.67%	
			25-14-200	0.207	0.197	0.0005	-4.83%	0.25%	
			24-19-340	0.347	0.331	0.0006	-4.61%	0.18%	
Linearity #3	9/15/2025	ALB	24-22-025	0.025	0.024	0.0004	-4.00%	1.67%	
			25-14-200	0.207	0.203	0.0008	-1.93%	0.39%	
			24-19-340	0.347	0.331	0.0006	-4.61%	0.18%	
0.01 g/210 L Acetone in 0.08 g/210L EtOH	9/10/2025	ALB	25-08-08A01	Int. Detected?	Yes				
0.02 g/210 L MeOH in H ₂ O	9/10/2025	ALB	25-18-00M02	Int. Detected?	Yes				
0.01 g/210 L IPA in H ₂ O	9/10/2025	ALB	25-03-00I01	Int. Detected?	Yes				

Tech Review:

9/18/25


Admin Review:

9/18/2025

Director Review:

9/18/2025

DMT Serial Number: 100146

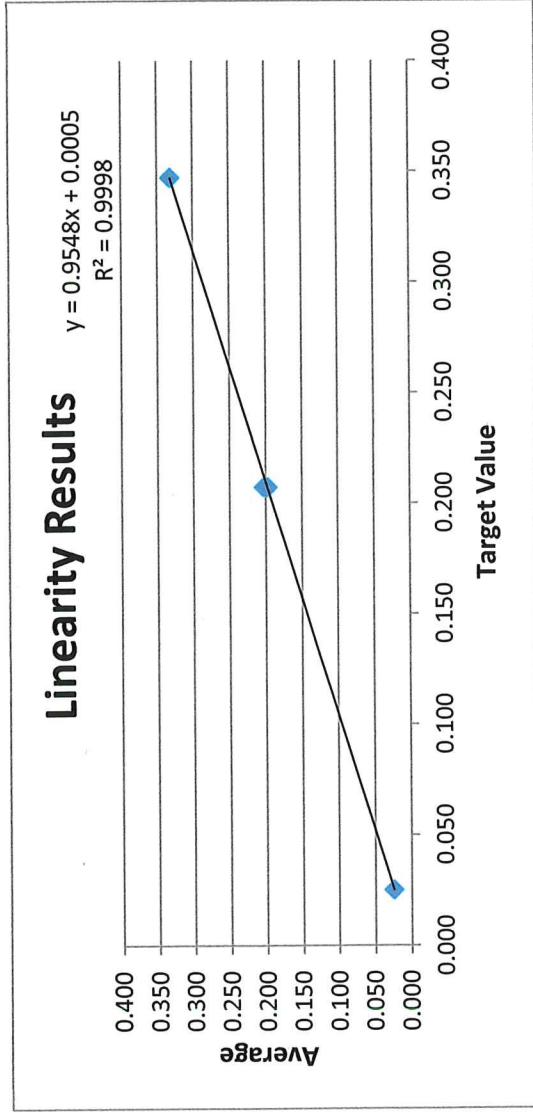

100146 ds 2



ACCURACY & PRECISION REPORT

STATE OF VERMONT

DataMaster DMT: 100146

Date: 9/10/2025

Time: 12:33:51


SUPERVISOR NAME:

AMANDA BOLDUC

SOLUTION LOT #: 25-18-00M02

SOLUTION CONCENTRATION: 0.020

BLANK TEST 0.000 12:34
SIMULATOR VAPOR 34.0°C INTERFERENCE 12:35
X[1] = 0.0140 (-0.0067) (-0.0039)
SIMULATOR VAPOR 34.0°C INTERFERENCE 12:36
X[1] = 0.0140 (-0.0070) (-0.0042)
SIMULATOR VAPOR 34.0°C INTERFERENCE 12:37
X[1] = 0.0141 (-0.0070) (-0.0048)
SIMULATOR VAPOR 34.0°C INTERFERENCE 12:38
X[1] = 0.0152 (-0.0068) (-0.0047)
SIMULATOR VAPOR 34.0°C INTERFERENCE 12:40
X[1] = 0.0146 (-0.0065) (-0.0044)
SIMULATOR VAPOR 34.0°C INTERFERENCE 12:41
X[1] = 0.0142 (-0.0074) (-0.0054)
SIMULATOR VAPOR 34.0°C INTERFERENCE 12:42
X[1] = 0.0143 (-0.0080) (-0.0039)
SIMULATOR VAPOR 34.0°C INTERFERENCE 12:44
X[1] = 0.0142 (-0.0068) (-0.0043)
SIMULATOR VAPOR 34.0°C INTERFERENCE 12:45
X[1] = 0.0140 (-0.0083) (-0.0052)
SIMULATOR VAPOR 34.0°C INTERFERENCE 12:46
X[1] = 0.0150 (-0.0074) (-0.0045)
BLANK TEST 0.000 12:47

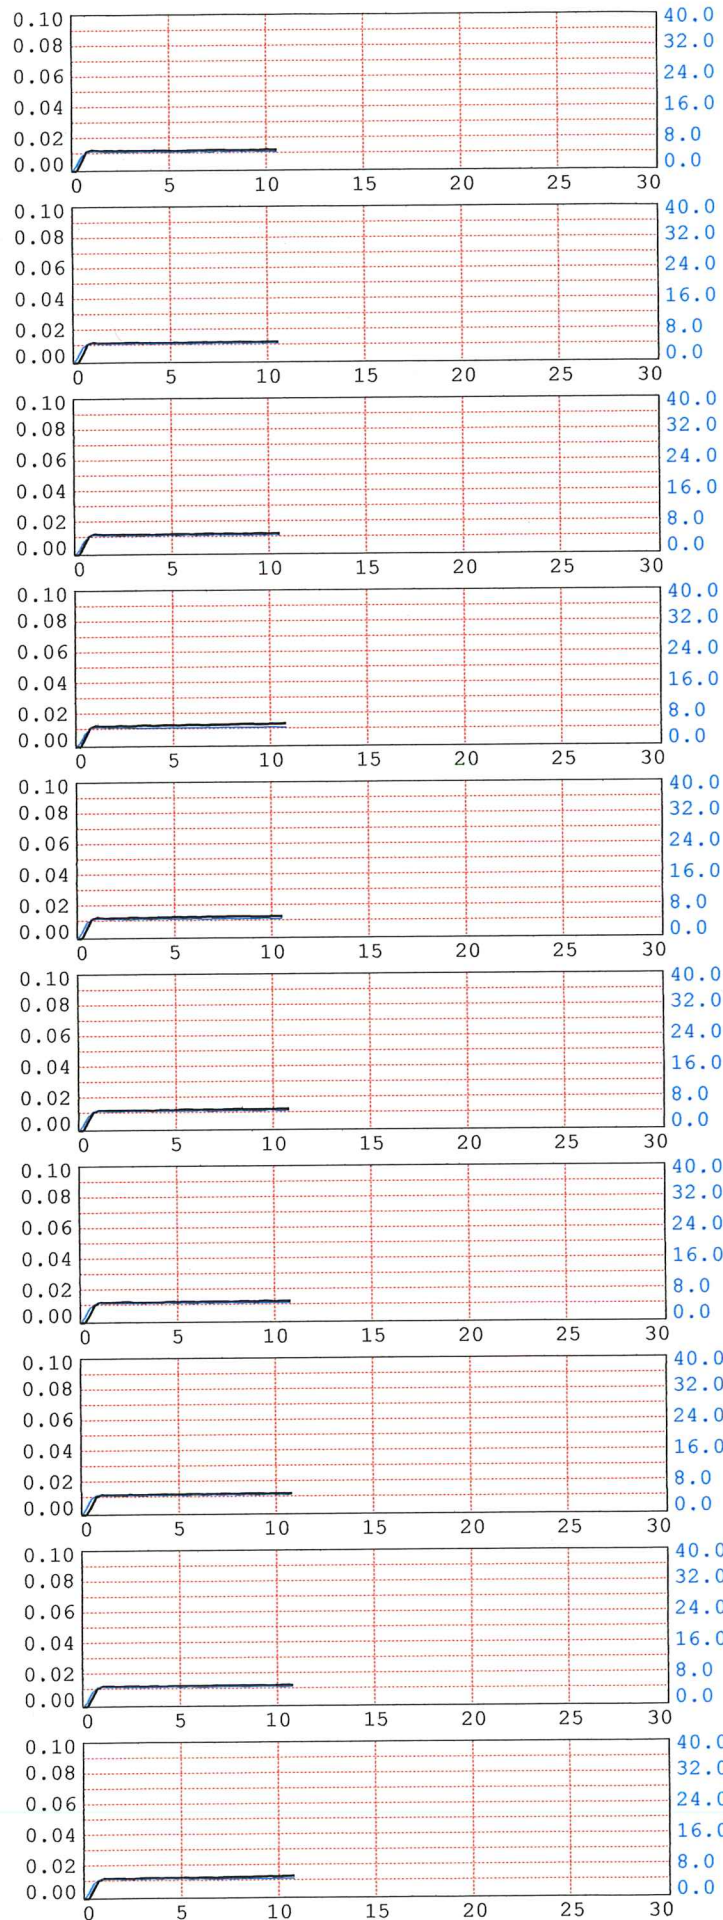

100146 AS 3



ACCURACY & PRECISION REPORT

STATE OF VERMONT

DataMaster DMT: 100146

Date: 9/10/2025

Time: 12:52:07


SUPERVISOR NAME:

AMANDA BOLDUC

SOLUTION LOT #: 25-03-00101

SOLUTION CONCENTRATION: 0.010

BLANK TEST 0.000 12:53
SIMULATOR VAPOR 34.0°C INTERFERENCE 12:53
X[1] = 0.0062 (-0.0065) (0.0028)
SIMULATOR VAPOR 34.0°C INTERFERENCE 12:54
X[1] = 0.0064 (-0.0070) (0.0016)
SIMULATOR VAPOR 34.0°C INTERFERENCE 12:55
X[1] = 0.0073 (-0.0060) (0.0015)
SIMULATOR VAPOR 34.0°C INTERFERENCE 12:57
X[1] = 0.0065 (-0.0065) (0.0021)
SIMULATOR VAPOR 34.0°C INTERFERENCE 12:58
X[1] = 0.0068 (-0.0063) (0.0023)
SIMULATOR VAPOR 34.0°C INTERFERENCE 12:59
X[1] = 0.0064 (-0.0063) (0.0019)
SIMULATOR VAPOR 34.0°C INTERFERENCE 13:00
X[1] = 0.0075 (-0.0062) (0.0017)
SIMULATOR VAPOR 34.0°C INTERFERENCE 13:01
X[1] = 0.0065 (-0.0067) (0.0021)
SIMULATOR VAPOR 34.0°C INTERFERENCE 13:03
X[1] = 0.0063 (-0.0065) (0.0024)
SIMULATOR VAPOR 34.0°C INTERFERENCE 13:04
X[1] = 0.0063 (-0.0065) (0.0004)
BLANK TEST 0.000 13:05

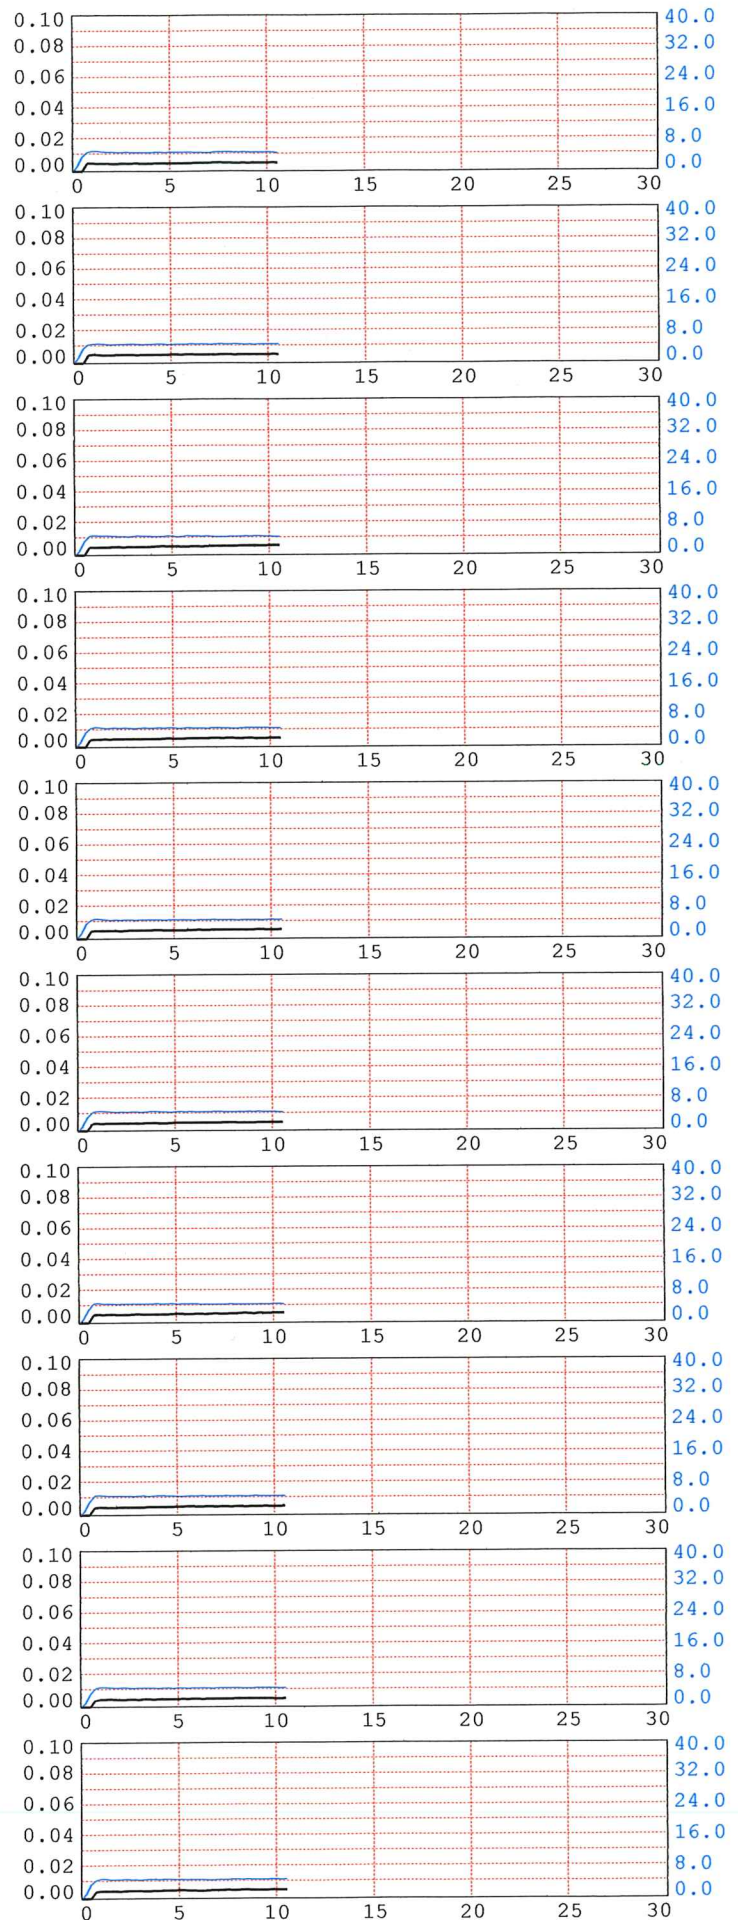

100146 AS 4



ACCURACY & PRECISION REPORT

STATE OF VERMONT

DataMaster DMT: 100146

Date: 9/10/2025

Time: 14:33:21


SUPERVISOR NAME:

AMANDA BOLDUC

SOLUTION LOT #: 25-08-08A01

SOLUTION CONCENTRATION: 0.010

BLANK TEST 0.000 14:34
SIMULATOR VAPOR 34.0°C INTERFERENCE 14:34
X[1] = 0.0823 (-0.0093) (0.0002)
SIMULATOR VAPOR 34.0°C INTERFERENCE 14:36
X[1] = 0.0827 (-0.0090) (0.0026)
SIMULATOR VAPOR 34.0°C INTERFERENCE 14:37
X[1] = 0.0827 (-0.0099) (-0.0001)
SIMULATOR VAPOR 34.0°C INTERFERENCE 14:38
X[1] = 0.0830 (-0.0098) (-0.0002)
SIMULATOR VAPOR 34.0°C INTERFERENCE 14:39
X[1] = 0.0828 (-0.0094) (0.0000)
SIMULATOR VAPOR 34.0°C INTERFERENCE 14:41
X[1] = 0.0829 (-0.0091) (-0.0019)
SIMULATOR VAPOR 34.0°C INTERFERENCE 14:42
X[1] = 0.0838 (-0.0089) (0.0004)
SIMULATOR VAPOR 34.0°C INTERFERENCE 14:44
X[1] = 0.0825 (-0.0095) (-0.0015)
SIMULATOR VAPOR 34.0°C INTERFERENCE 14:45
X[1] = 0.0827 (-0.0076) (0.0034)
SIMULATOR VAPOR 34.0°C INTERFERENCE 14:47
X[1] = 0.0820 (-0.0099) (-0.0001)
BLANK TEST 0.000 14:48

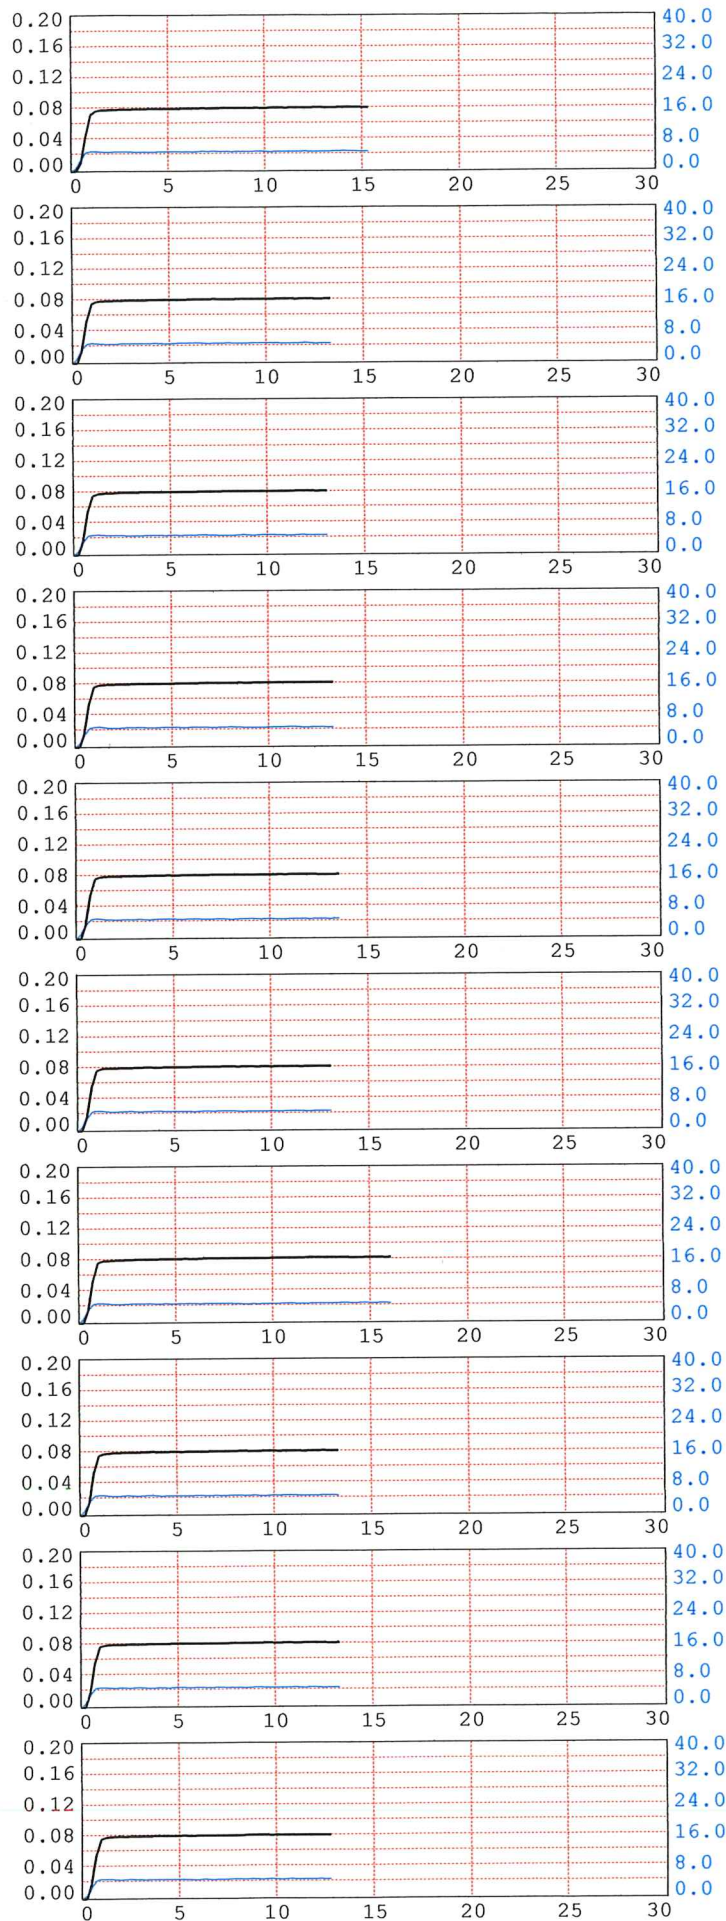

100146 AS 5



ACCURACY & PRECISION REPORT

STATE OF VERMONT

DataMaster DMT: 100146

Date: 9/11/2025

Time: 07:50:47


SUPERVISOR NAME:
AMANDA BOLDUC

SOLUTION LOT #: 24-22-025

SOLUTION CONCENTRATION: 0.025

BLANK TEST	0.000	07:51
SIMULATOR VAPOR 34.0°C	0.024	07:52
X[1] = 0.0239 (0.0001) (0.0014)		
SIMULATOR VAPOR 34.0°C	0.024	07:53
X[1] = 0.0238 (0.0007) (-0.0001)		
SIMULATOR VAPOR 34.0°C	0.024	07:54
X[1] = 0.0244 (-0.0005) (0.0005)		
SIMULATOR VAPOR 34.0°C	0.024	07:55
X[1] = 0.0238 (-0.0008) (-0.0004)		
SIMULATOR VAPOR 34.0°C	0.024	07:57
X[1] = 0.0243 (-0.0005) (0.0006)		
SIMULATOR VAPOR 34.0°C	0.024	07:58
X[1] = 0.0244 (0.0004) (0.0002)		
SIMULATOR VAPOR 34.0°C	0.024	07:59
X[1] = 0.0243 (0.0004) (0.0003)		
SIMULATOR VAPOR 34.0°C	0.024	08:00
X[1] = 0.0241 (-0.0008) (-0.0023)		
SIMULATOR VAPOR 34.0°C	0.024	08:01
X[1] = 0.0241 (-0.0009) (0.0004)		
SIMULATOR VAPOR 34.0°C	0.024	08:03
X[1] = 0.0240 (-0.0011) (0.0002)		
BLANK TEST	0.000	08:04

Average = 0.024
Std Dev = 0.0002

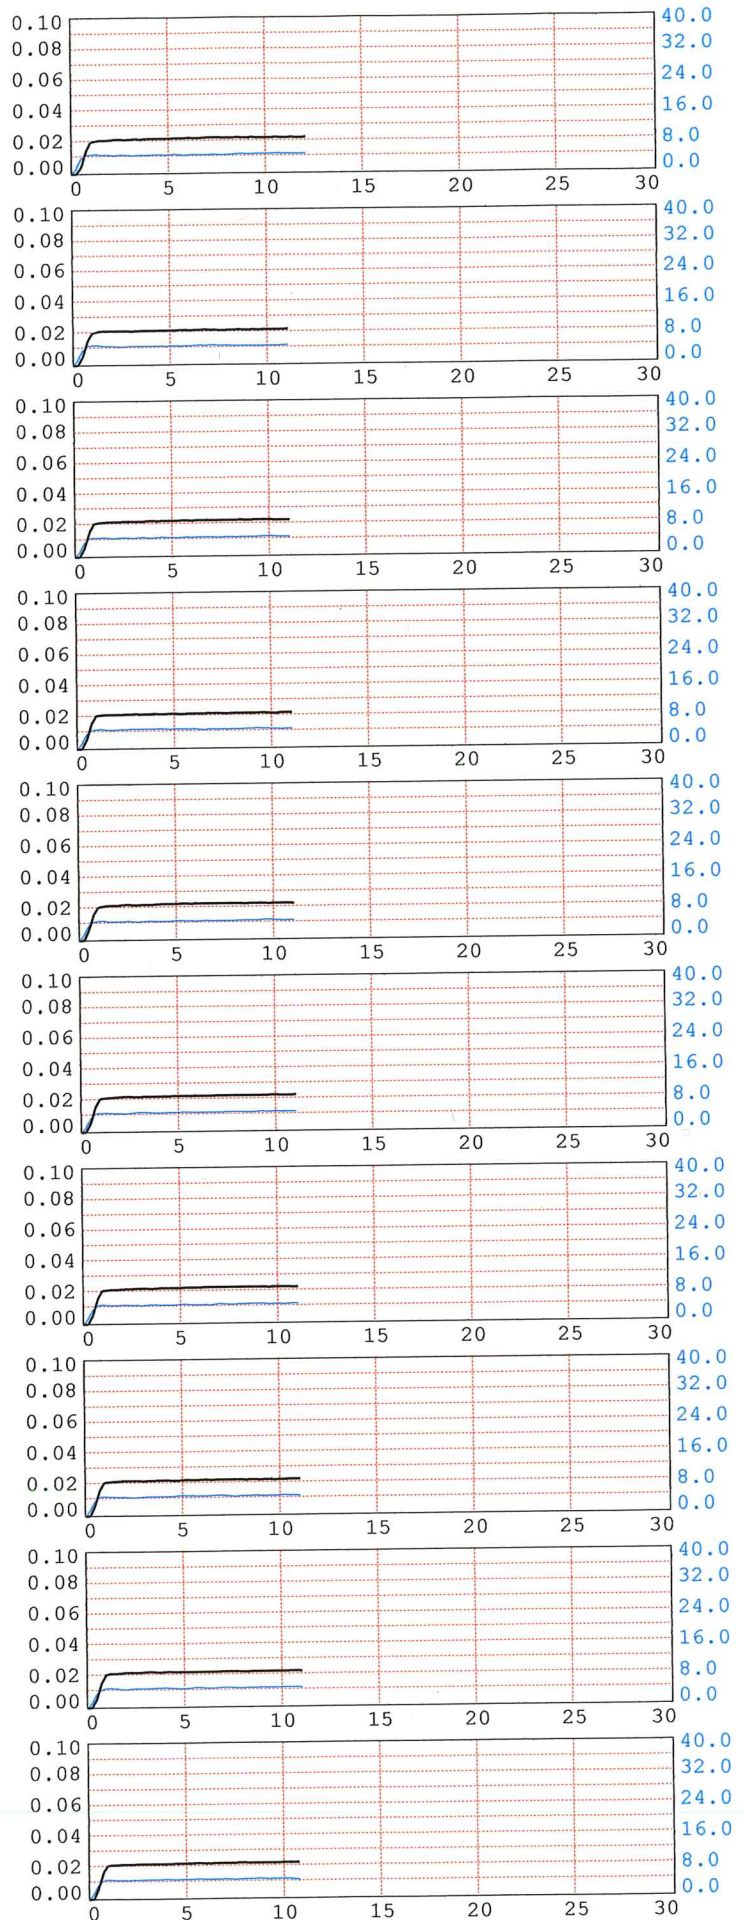

100146 AB 6



ACCURACY & PRECISION REPORT

STATE OF VERMONT

DataMaster DMT: 100146

Date: 9/11/2025

Time: 08:12:01

SUPERVISOR NAME:

AMANDA BOLDUC


SOLUTION LOT #: 25-14-200

SOLUTION CONCENTRATION: 0.207

BLANK TEST	0.000	08:13
SIMULATOR VAPOR 34.0°C	0.198	08:13
X[1] = 0.1976 (0.0009) (0.0028)		
SIMULATOR VAPOR 34.0°C	0.198	08:14
X[1] = 0.1976 (0.0005) (0.0018)		
SIMULATOR VAPOR 34.0°C	0.197	08:16
X[1] = 0.1973 (0.0006) (0.0016)		
SIMULATOR VAPOR 34.0°C	0.197	08:17
X[1] = 0.1972 (0.0008) (0.0014)		
SIMULATOR VAPOR 34.0°C	0.197	08:18
X[1] = 0.1974 (0.0008) (0.0017)		
SIMULATOR VAPOR 34.0°C	0.197	08:20
X[1] = 0.1971 (0.0013) (0.0008)		
SIMULATOR VAPOR 34.0°C	0.197	08:21
X[1] = 0.1971 (-0.0002) (0.0007)		
SIMULATOR VAPOR 34.0°C	0.198	08:22
X[1] = 0.1975 (0.0002) (-0.0009)		
SIMULATOR VAPOR 34.0°C	0.198	08:24
X[1] = 0.1979 (0.0008) (0.0009)		
SIMULATOR VAPOR 34.0°C	0.198	08:25
X[1] = 0.1977 (0.0005) (0.0015)		
BLANK TEST	0.000	08:26

Average = 0.197

Std Dev = 0.0003

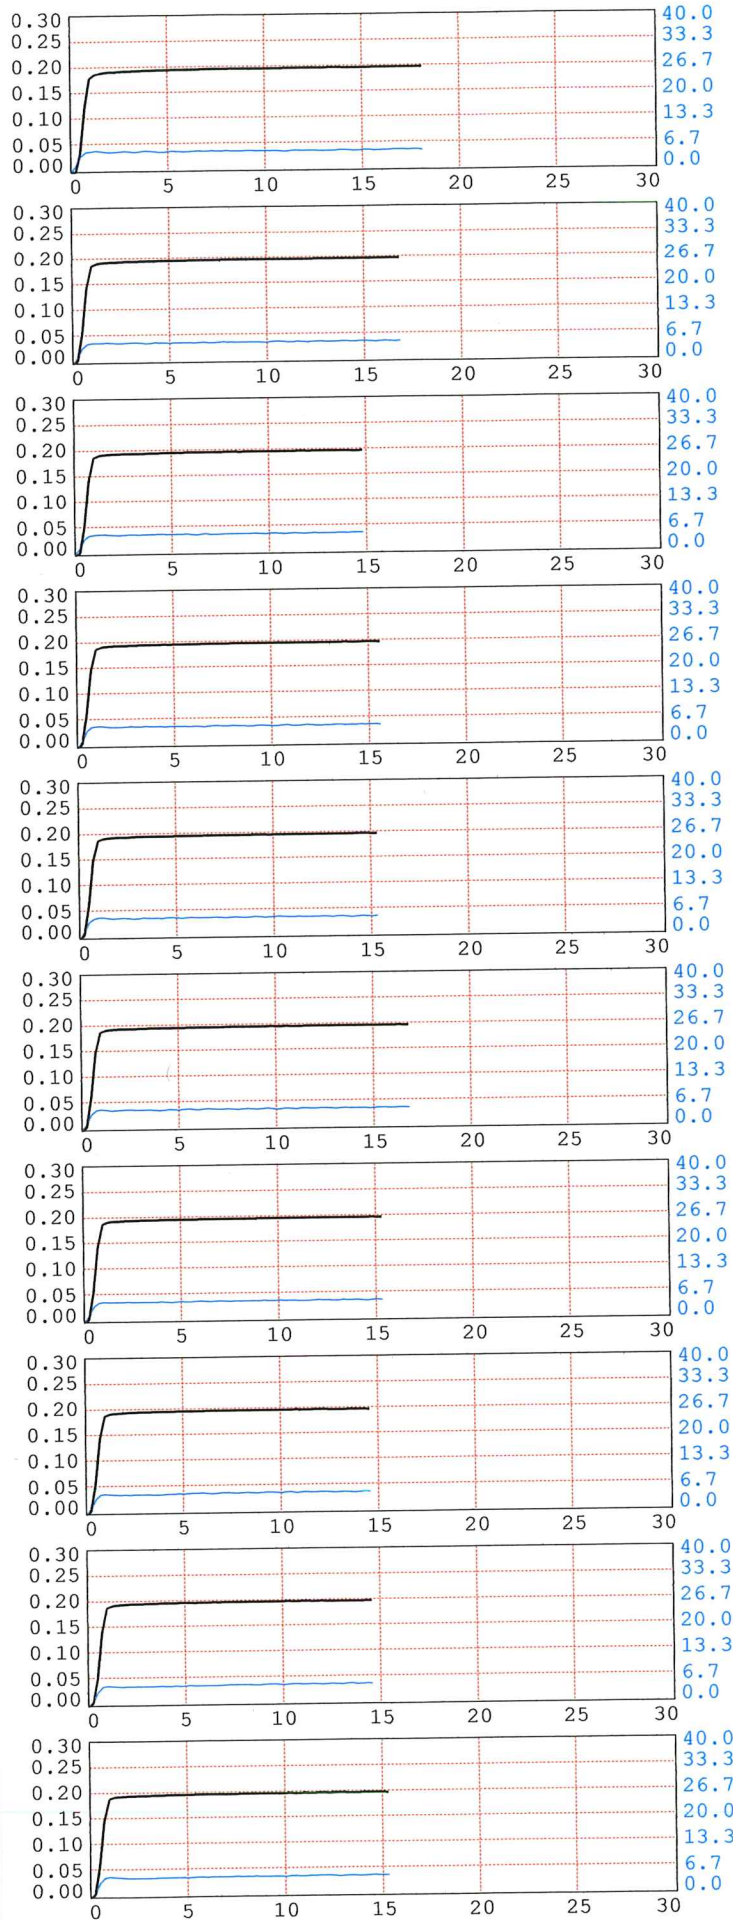

100146 ds 7



ACCURACY & PRECISION REPORT

STATE OF VERMONT

DataMaster DMT: 100146

Date: 9/11/2025

Time: 08:33:17

SUPERVISOR NAME:

AMANDA BOLDUC


SOLUTION LOT #: 24-19-340

SOLUTION CONCENTRATION: 0.347

BLANK TEST	0.000	08:34
SIMULATOR VAPOR 34.0°C	0.332	08:34
X[1] = 0.3325 (0.0024) (0.0033)		
SIMULATOR VAPOR 34.0°C	0.332	08:36
X[1] = 0.3325 (0.0027) (0.0016)		
SIMULATOR VAPOR 34.0°C	0.333	08:37
X[1] = 0.3327 (0.0022) (0.0024)		
SIMULATOR VAPOR 34.0°C	0.332	08:38
X[1] = 0.3322 (0.0017) (0.0024)		
SIMULATOR VAPOR 34.0°C	0.332	08:40
X[1] = 0.3320 (0.0018) (0.0028)		
SIMULATOR VAPOR 34.0°C	0.333	08:41
X[1] = 0.3326 (0.0022) (0.0023)		
SIMULATOR VAPOR 34.0°C	0.332	08:43
X[1] = 0.3324 (0.0015) (0.0024)		
SIMULATOR VAPOR 34.0°C	0.332	08:44
X[1] = 0.3324 (0.0022) (0.0026)		
SIMULATOR VAPOR 34.0°C	0.332	08:45
X[1] = 0.3323 (0.0020) (0.0030)		
SIMULATOR VAPOR 34.0°C	0.333	08:47
X[1] = 0.3327 (0.0025) (0.0053)		
BLANK TEST	0.000	08:48

Average = 0.332

Std Dev = 0.0002

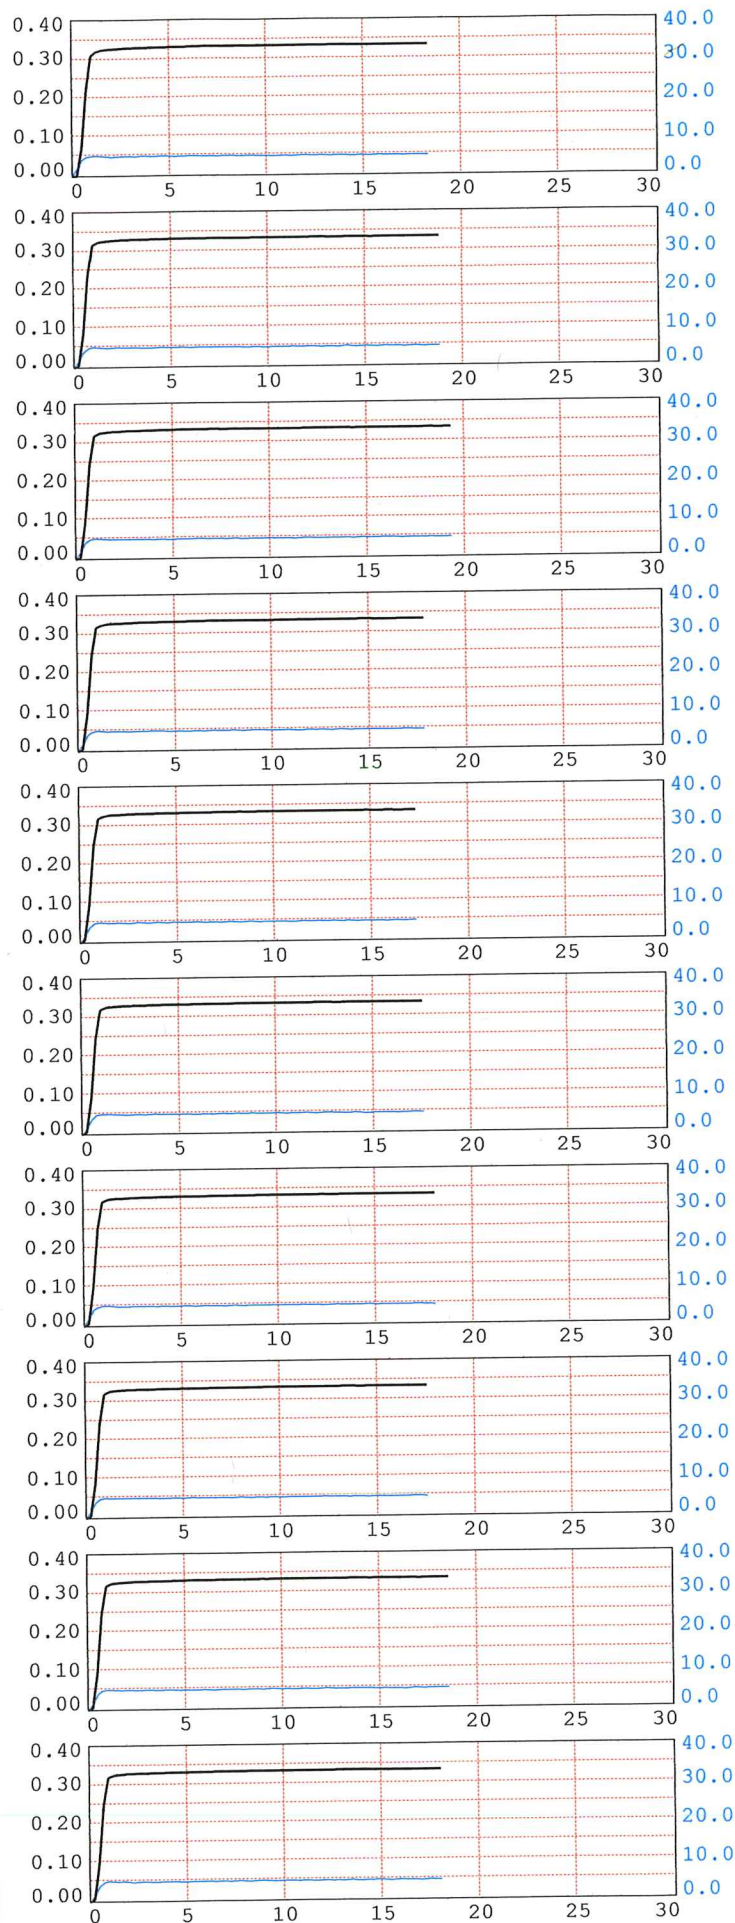

100146 AS 8



ACCURACY & PRECISION REPORT

STATE OF VERMONT

DataMaster DMT: 100146

Date: 9/12/2025

Time: 07:28:21

SUPERVISOR NAME:
AMANDA BOLDUC


SOLUTION LOT #: 24-22-025

SOLUTION CONCENTRATION: 0.025

BLANK TEST	0.000	07:29
SIMULATOR VAPOR 34.0°C	0.022	07:29
X[1] = 0.0225 (0.0006) (0.0006)		
SIMULATOR VAPOR 34.0°C	0.024	07:30
X[1] = 0.0238 (-0.0008) (-0.0001)		
SIMULATOR VAPOR 34.0°C	0.024	07:32
X[1] = 0.0237 (-0.0005) (0.0004)		
SIMULATOR VAPOR 34.0°C	0.024	07:33
X[1] = 0.0240 (0.0003) (-0.0003)		
SIMULATOR VAPOR 34.0°C	0.024	07:34
X[1] = 0.0238 (-0.0004) (-0.0003)		
SIMULATOR VAPOR 34.0°C	0.024	07:35
X[1] = 0.0237 (0.0002) (-0.0001)		
SIMULATOR VAPOR 34.0°C	0.024	07:37
X[1] = 0.0237 (-0.0006) (-0.0004)		
SIMULATOR VAPOR 34.0°C	0.024	07:38
X[1] = 0.0238 (0.0005) (-0.0002)		
SIMULATOR VAPOR 34.0°C	0.024	07:39
X[1] = 0.0238 (-0.0005) (-0.0004)		
SIMULATOR VAPOR 34.0°C	0.024	07:40
X[1] = 0.0236 (-0.0006) (0.0000)		
BLANK TEST	0.000	07:41

Average = 0.024

Std Dev = 0.0004

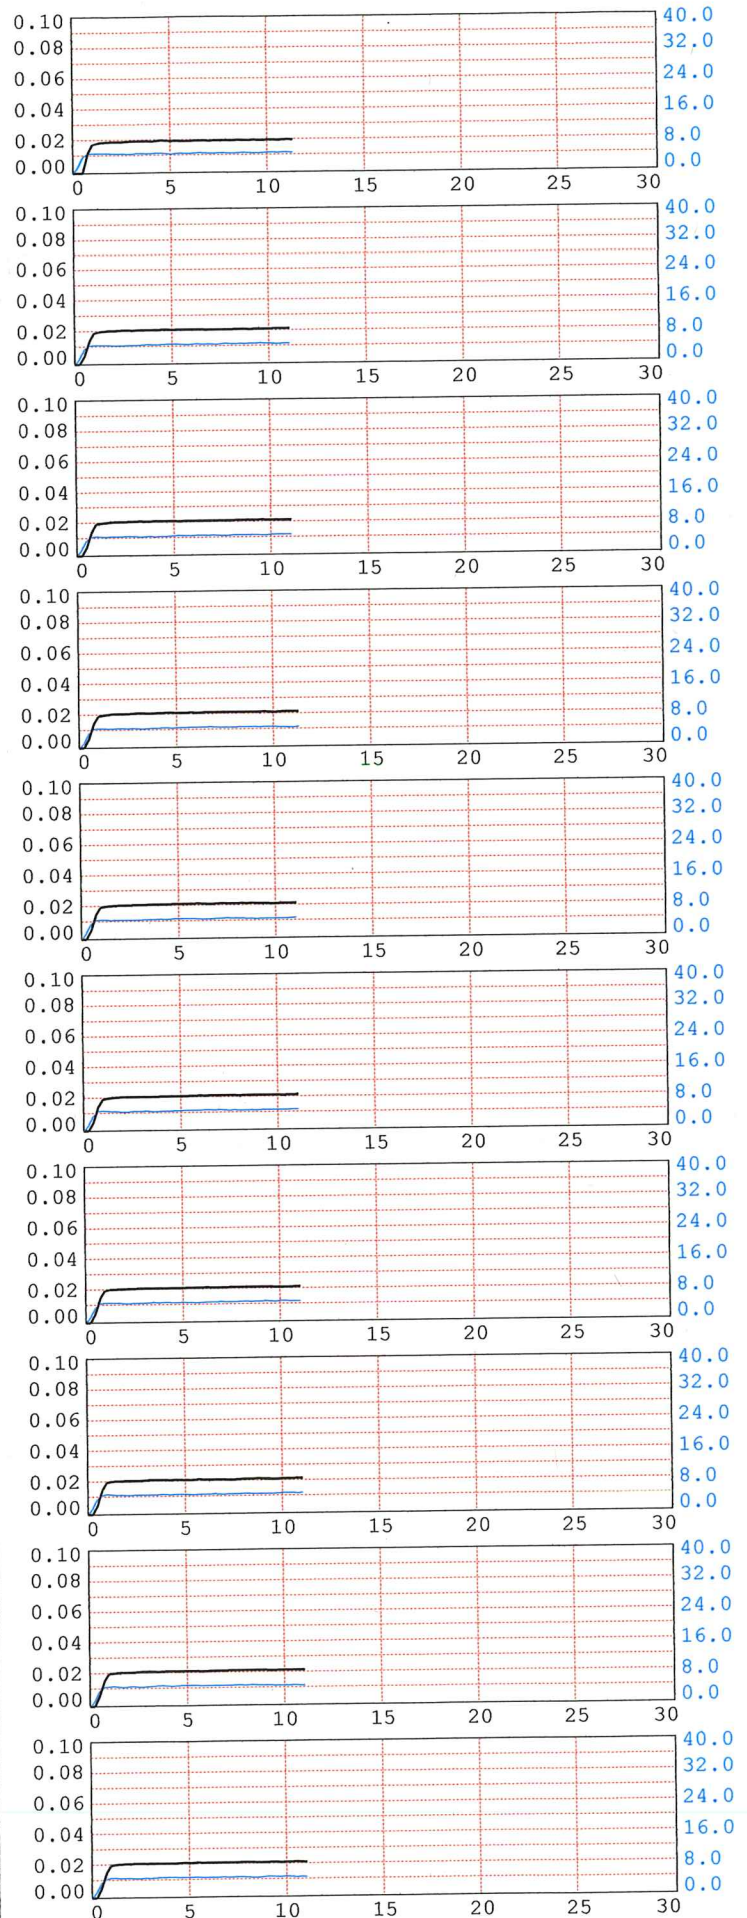

100146 25 9



ACCURACY & PRECISION REPORT

STATE OF VERMONT

DataMaster DMT: 100146

Date: 9/12/2025

Time: 09:33:32


SUPERVISOR NAME:
AMANDA BOLDUC

SOLUTION LOT #: 25-14-200

SOLUTION CONCENTRATION: 0.207

BLANK TEST	0.000	09:34
SIMULATOR VAPOR 34.0°C	0.197	09:34
X[1] = 0.1971 (0.0006) (0.0007)		
SIMULATOR VAPOR 34.0°C	0.198	09:36
X[1] = 0.1977 (0.0001) (-0.0001)		
SIMULATOR VAPOR 34.0°C	0.196	09:37
X[1] = 0.1964 (-0.0002) (-0.0010)		
SIMULATOR VAPOR 34.0°C	0.196	09:39
X[1] = 0.1965 (0.0000) (-0.0002)		
SIMULATOR VAPOR 34.0°C	0.196	09:40
X[1] = 0.1964 (0.0009) (-0.0025)		
SIMULATOR VAPOR 34.0°C	0.196	09:41
X[1] = 0.1963 (-0.0002) (-0.0003)		
SIMULATOR VAPOR 34.0°C	0.196	09:43
X[1] = 0.1963 (0.0004) (-0.0023)		
SIMULATOR VAPOR 34.0°C	0.196	09:44
X[1] = 0.1963 (0.0001) (0.0001)		
SIMULATOR VAPOR 34.0°C	0.196	09:45
X[1] = 0.1963 (0.0010) (-0.0002)		
SIMULATOR VAPOR 34.0°C	0.196	09:46
X[1] = 0.1965 (0.0013) (-0.0023)		
BLANK TEST	0.000	09:48

Average = 0.197
Std Dev = 0.0005

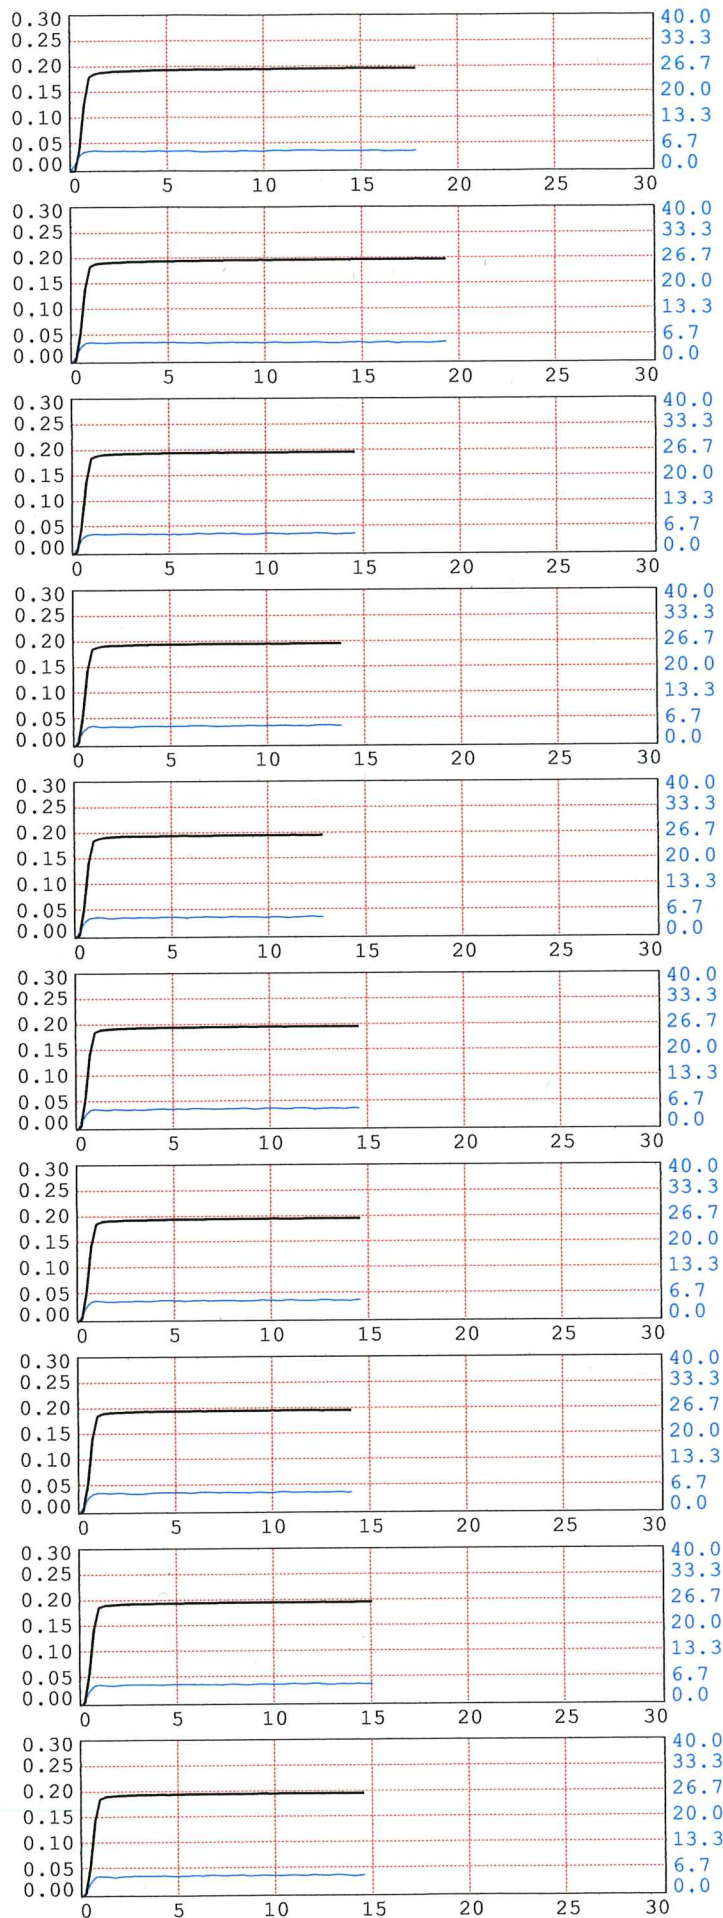

100146 *AB* 10



ACCURACY & PRECISION REPORT

STATE OF VERMONT

DataMaster DMT: 100146

Date: 9/12/2025

Time: 10:06:12

SUPERVISOR NAME:

AMANDA BOLDUC


SOLUTION LOT #: 24-19-340

SOLUTION CONCENTRATION: 0.347

BLANK TEST	0.000	10:07
SIMULATOR VAPOR 34.0°C	0.332	10:07
X[1] = 0.3321 (0.0017) (0.0014)		
SIMULATOR VAPOR 34.0°C	0.332	10:09
X[1] = 0.3325 (0.0022) (0.0010)		
SIMULATOR VAPOR 34.0°C	0.332	10:10
X[1] = 0.3320 (0.0031) (0.0015)		
SIMULATOR VAPOR 34.0°C	0.331	10:12
X[1] = 0.3314 (0.0023) (0.0005)		
SIMULATOR VAPOR 34.0°C	0.331	10:13
X[1] = 0.3312 (0.0016) (0.0001)		
SIMULATOR VAPOR 34.0°C	0.331	10:15
X[1] = 0.3312 (0.0012) (0.0003)		
SIMULATOR VAPOR 34.0°C	0.331	10:16
X[1] = 0.3306 (0.0006) (0.0001)		
SIMULATOR VAPOR 34.0°C	0.331	10:17
X[1] = 0.3313 (0.0016) (-0.0019)		
SIMULATOR VAPOR 34.0°C	0.331	10:19
X[1] = 0.3314 (0.0013) (0.0008)		
SIMULATOR VAPOR 34.0°C	0.331	10:20
X[1] = 0.3312 (0.0021) (0.0012)		
BLANK TEST	0.000	10:21

Average = 0.331

Std Dev = 0.0006

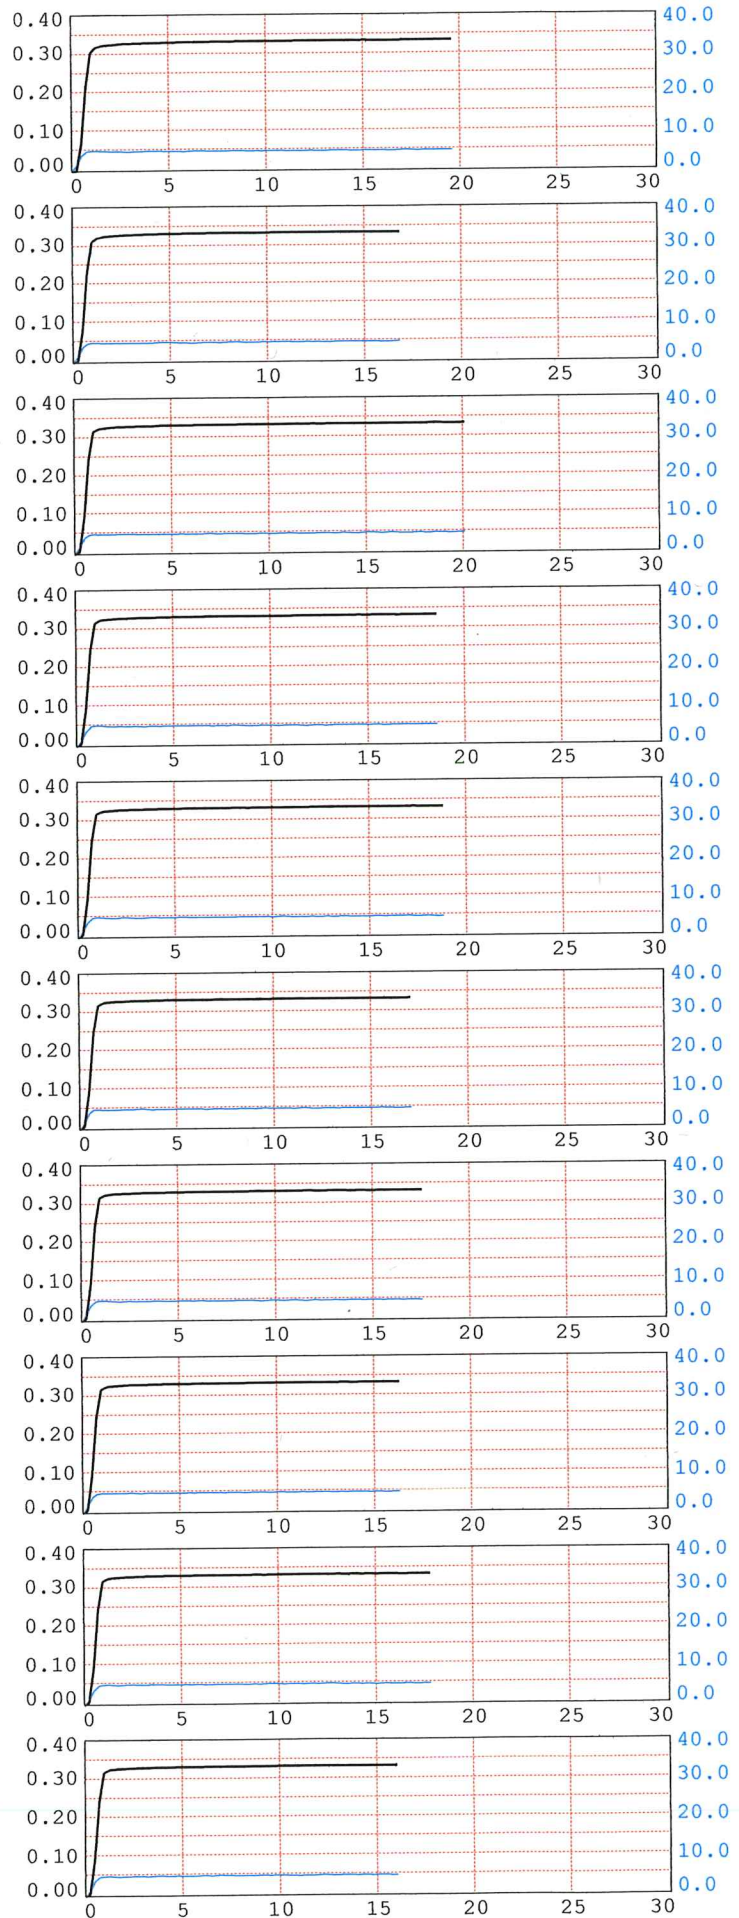

100146 *ds* 11



ACCURACY & PRECISION REPORT

STATE OF VERMONT

DataMaster DMT: 100146

Date: 9/15/2025

Time: 07:44:44

SUPERVISOR NAME:

AMANDA BOLDUC


SOLUTION LOT #: 24-22-025

SOLUTION CONCENTRATION: 0.025

BLANK TEST	0.000	07:45
SIMULATOR VAPOR 34.0°C	0.023	07:46
X[1] = 0.0232 (0.0008) (0.0019)		
SIMULATOR VAPOR 34.0°C	0.023	07:47
X[1] = 0.0234 (-0.0007) (0.0007)		
SIMULATOR VAPOR 34.0°C	0.024	07:48
X[1] = 0.0242 (0.0007) (-0.0002)		
SIMULATOR VAPOR 34.0°C	0.024	07:49
X[1] = 0.0239 (0.0008) (0.0002)		
SIMULATOR VAPOR 34.0°C	0.024	07:50
X[1] = 0.0245 (-0.0007) (0.0005)		
SIMULATOR VAPOR 34.0°C	0.024	07:52
X[1] = 0.0238 (-0.0012) (0.0002)		
SIMULATOR VAPOR 34.0°C	0.024	07:53
X[1] = 0.0240 (-0.0010) (0.0004)		
SIMULATOR VAPOR 34.0°C	0.024	07:54
X[1] = 0.0237 (0.0009) (0.0002)		
SIMULATOR VAPOR 34.0°C	0.024	07:55
X[1] = 0.0245 (0.0012) (0.0005)		
SIMULATOR VAPOR 34.0°C	0.024	07:57
X[1] = 0.0243 (0.0005) (0.0007)		
BLANK TEST	0.000	07:58

Average = 0.024

Std Dev = 0.0004

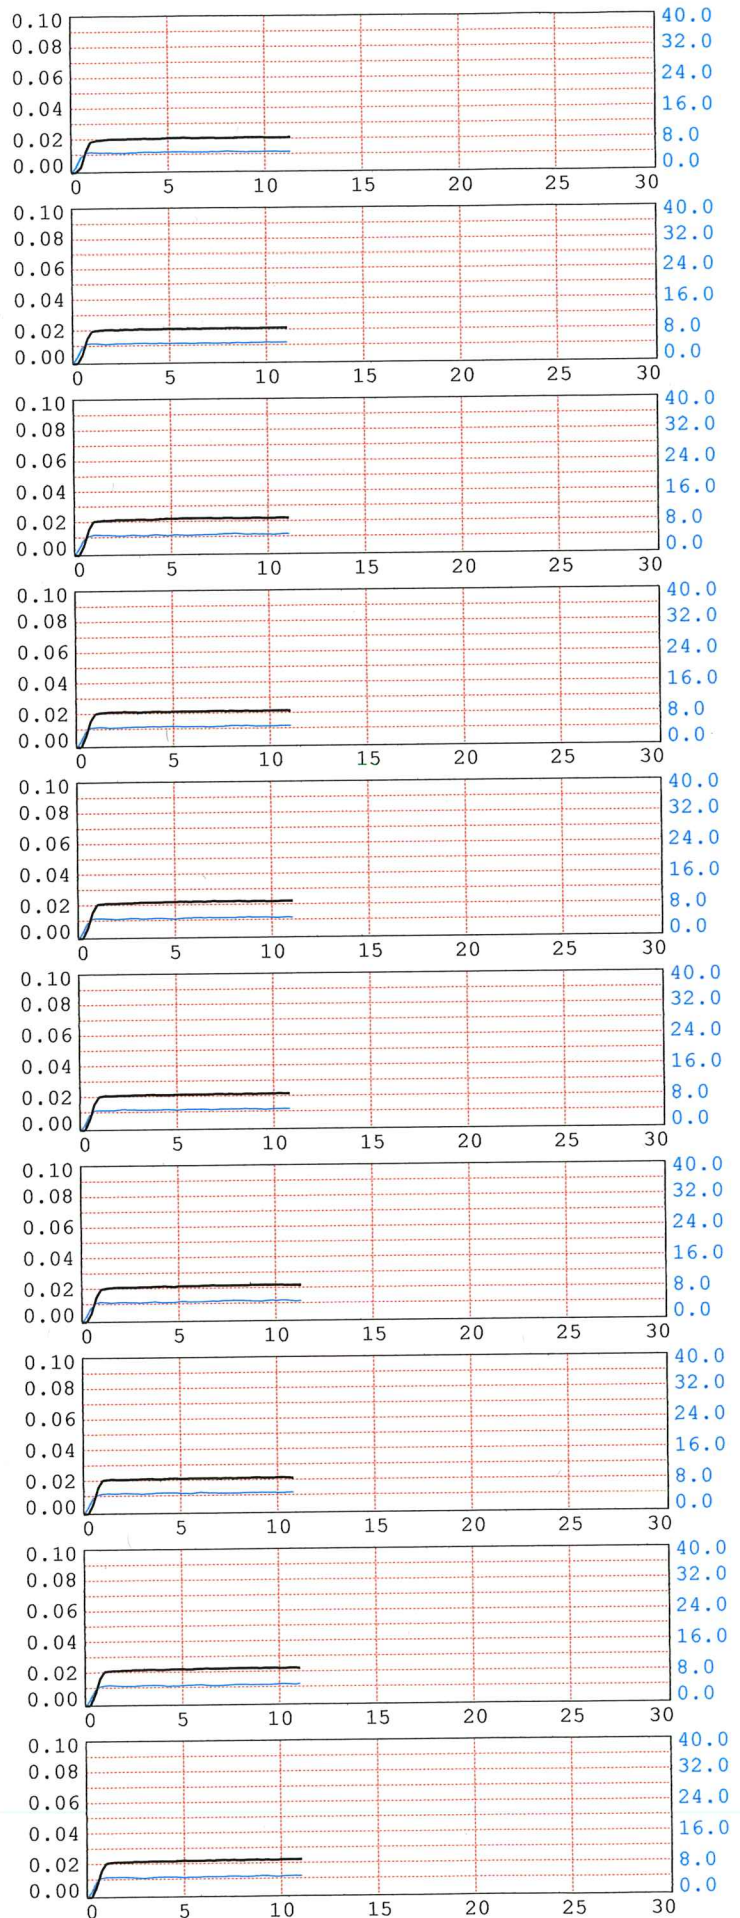

100146 OK 12



ACCURACY & PRECISION REPORT

STATE OF VERMONT

DataMaster DMT: 100146

Date: 9/15/2025

Time: 08:17:44

SUPERVISOR NAME:

AMANDA BOLDUC

SOLUTION LOT #: 25-14-200


SOLUTION CONCENTRATION: 0.207

BLANK TEST	0.000	08:18
SIMULATOR VAPOR 34.0°C	0.195	08:19
X[1] = 0.1952 (0.0010) (0.0043)		
SIMULATOR VAPOR 34.0°C	0.197	08:20
X[1] = 0.1968 (0.0010) (-0.0002)		
SIMULATOR VAPOR 34.0°C	0.196	08:21
X[1] = 0.1964 (0.0008) (0.0015)		
SIMULATOR VAPOR 34.0°C	0.196	08:23
X[1] = 0.1961 (0.0005) (0.0011)		
SIMULATOR VAPOR 34.0°C	0.196	08:24
X[1] = 0.1959 (0.0012) (0.0001)		
SIMULATOR VAPOR 34.0°C	0.196	08:26
X[1] = 0.1957 (0.0002) (0.0007)		
SIMULATOR VAPOR 34.0°C	0.196	08:27
X[1] = 0.1956 (-0.0004) (0.0007)		
SIMULATOR VAPOR 34.0°C	0.196	08:28
X[1] = 0.1957 (0.0014) (0.0008)		
SIMULATOR VAPOR 34.0°C	0.196	08:30
X[1] = 0.1957 (0.0002) (0.0009)		
SIMULATOR VAPOR 34.0°C	0.196	08:31
X[1] = 0.1956 (0.0005) (0.0006)		
BLANK TEST	0.000	08:32

Average = 0.196

Std Dev = 0.0005

*out of
range -
re-run* *AS*
9/15/25

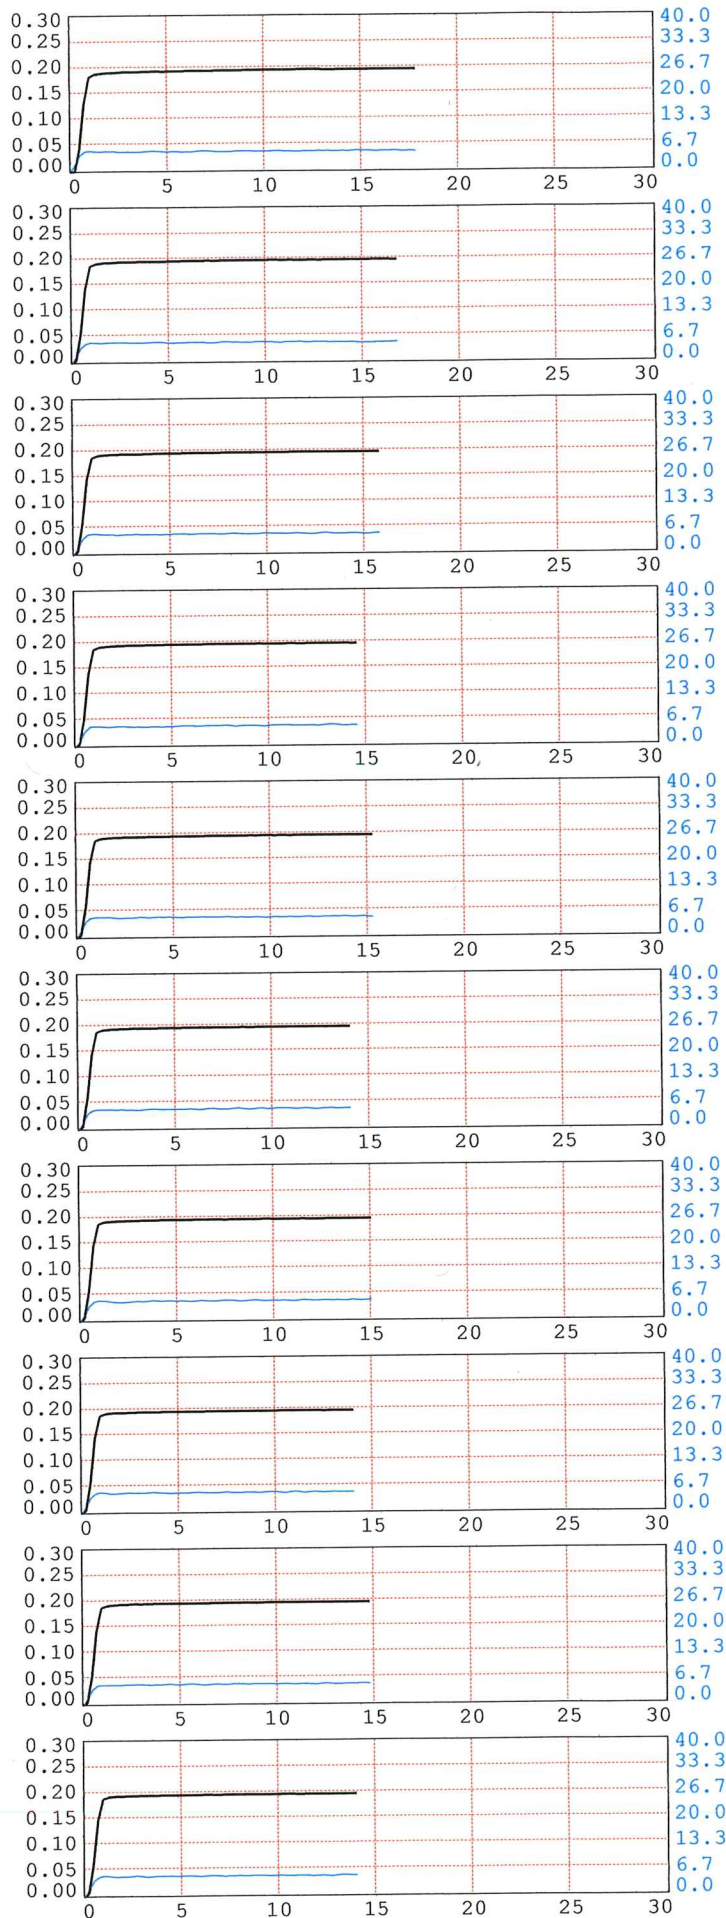

100146 AS 13



ACCURACY & PRECISION REPORT

STATE OF VERMONT

DataMaster DMT: 100146

Date: 9/15/2025

Time: 08:33:49

SUPERVISOR NAME:

AMANDA BOLDUC



SOLUTION LOT #: 25-14-200

SOLUTION CONCENTRATION: 0.207

BLANK TEST	0.000	08:34
SIMULATOR VAPOR 34.0°C	0.196	08:35
SIMULATOR VAPOR 34.0°C	0.196	08:36

User Abort

*failing low
solution changed
AS
9/15/25*

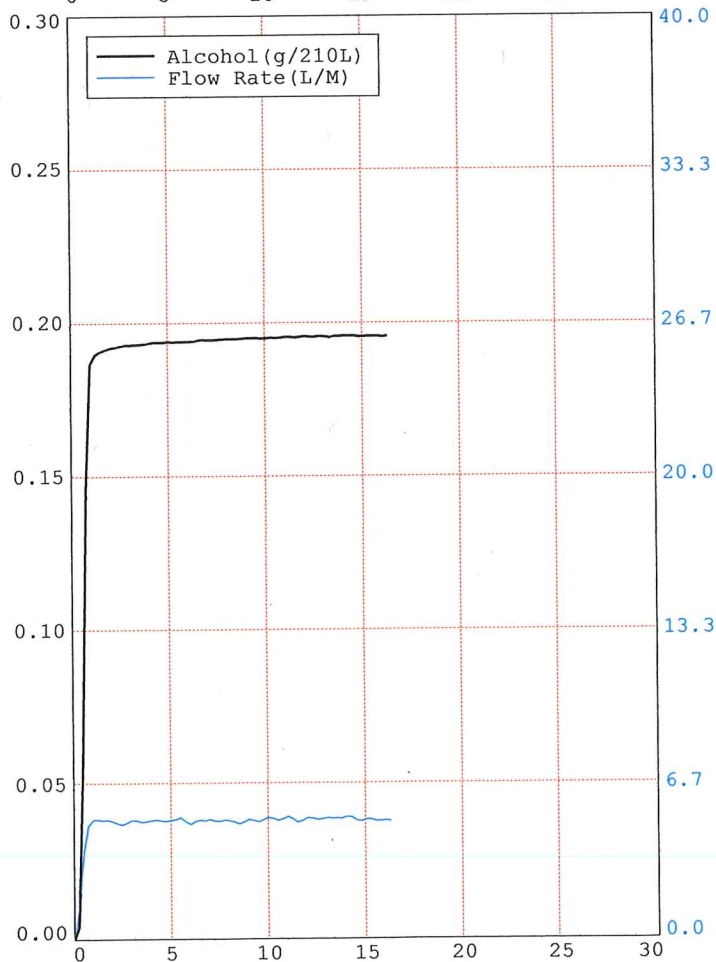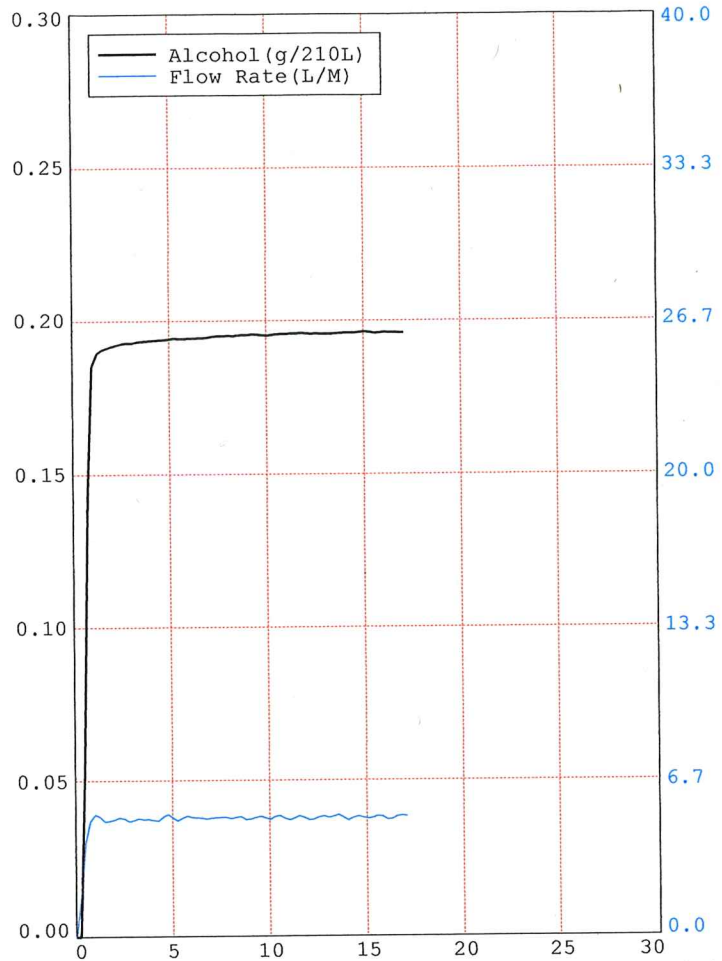

100146 AS 149



ACCURACY & PRECISION REPORT

STATE OF VERMONT

DataMaster DMT: 100146

Date: 9/15/2025

Time: 10:26:46

SUPERVISOR NAME:

AMANDA BOLDUC


SOLUTION LOT #: 25-14-200

SOLUTION CONCENTRATION: 0.207

BLANK TEST	0.000	10:27
SIMULATOR VAPOR 34.0°C	0.205	10:28
SIMULATOR VAPOR 34.0°C	0.204	10:29
SIMULATOR VAPOR 34.0°C	0.203	10:31
SIMULATOR VAPOR 34.0°C	0.203	10:32
SIMULATOR VAPOR 34.0°C	0.202	10:34
SIMULATOR VAPOR 34.0°C	0.202	10:35
SIMULATOR VAPOR 34.0°C	0.203	10:36
SIMULATOR VAPOR 34.0°C	0.202	10:38
SIMULATOR VAPOR 34.0°C	0.202	10:39
SIMULATOR VAPOR 34.0°C	0.202	10:40
BLANK TEST	0.000	10:41

Average = 0.203

Std Dev = 0.0008

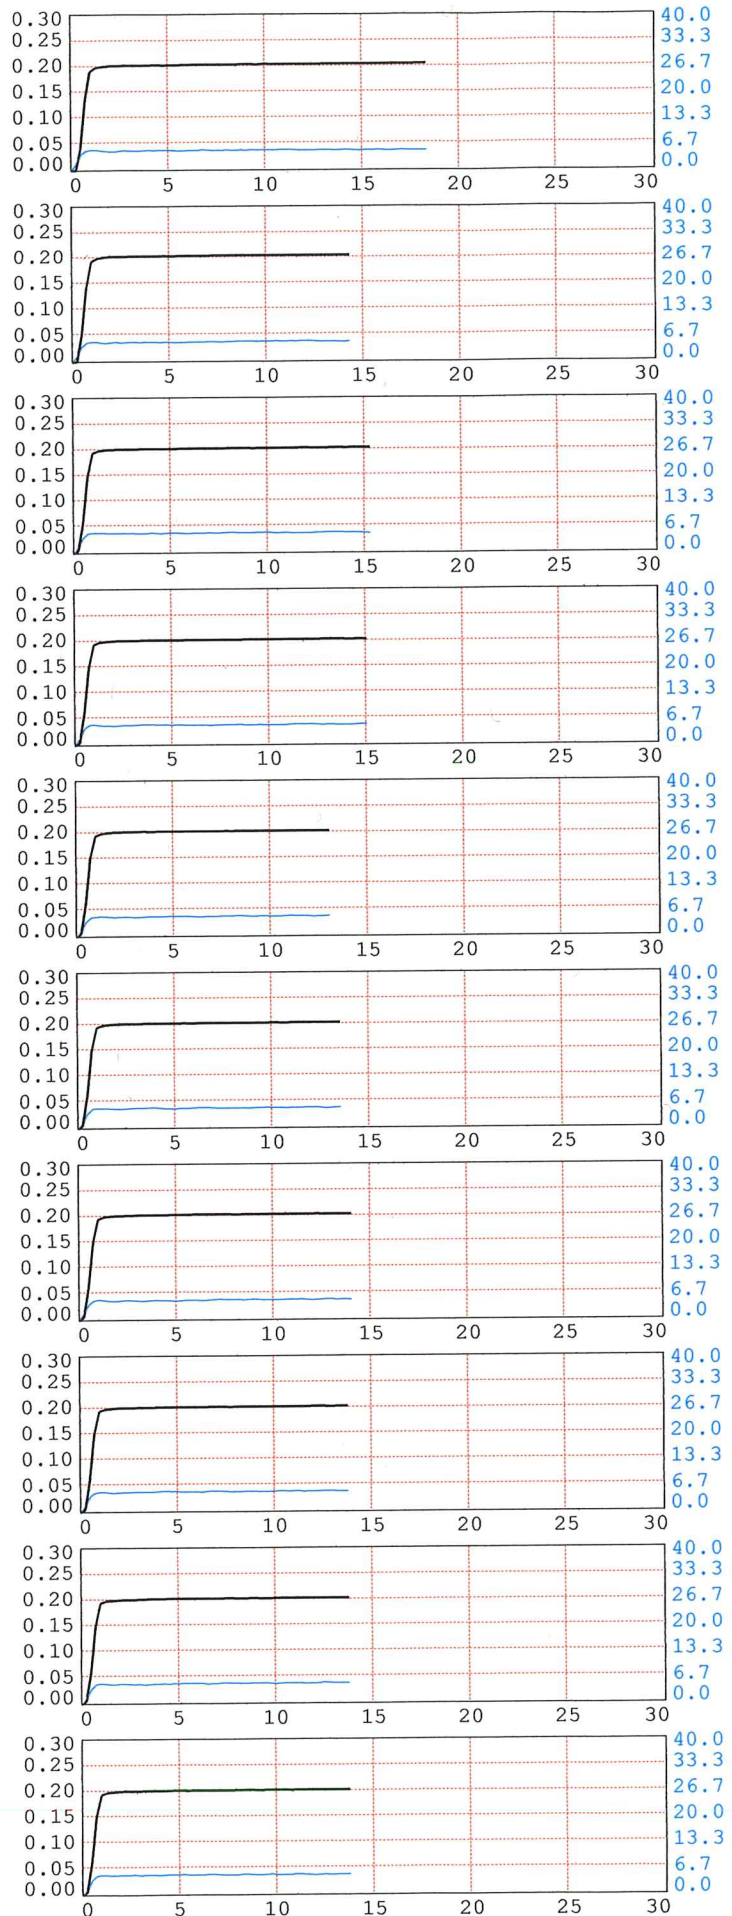

100146 AS 15



ACCURACY & PRECISION REPORT

STATE OF VERMONT

DataMaster DMT: 100146

Date: 9/15/2025

Time: 10:43:39


SUPERVISOR NAME:
AMANDA BOLDUC

SOLUTION LOT #: 24-19-340

SOLUTION CONCENTRATION: 0.347

BLANK TEST	0.000	10:44
SIMULATOR VAPOR 34.0°C	0.332	10:45
X[1] = 0.3320 (-0.0007) (0.0025)		
SIMULATOR VAPOR 34.0°C	0.331	10:46
X[1] = 0.3309 (0.0011) (-0.0011)		
SIMULATOR VAPOR 34.0°C	0.330	10:47
X[1] = 0.3304 (-0.0008) (-0.0018)		
SIMULATOR VAPOR 34.0°C	0.330	10:49
X[1] = 0.3304 (0.0004) (-0.0012)		
SIMULATOR VAPOR 34.0°C	0.330	10:50
X[1] = 0.3304 (0.0004) (0.0006)		
SIMULATOR VAPOR 34.0°C	0.330	10:51
X[1] = 0.3304 (-0.0002) (0.0009)		
SIMULATOR VAPOR 34.0°C	0.331	10:53
X[1] = 0.3306 (0.0002) (0.0006)		
SIMULATOR VAPOR 34.0°C	0.330	10:54
X[1] = 0.3304 (-0.0002) (0.0014)		
SIMULATOR VAPOR 34.0°C	0.330	10:55
X[1] = 0.3299 (-0.0001) (0.0008)		
SIMULATOR VAPOR 34.0°C	0.330	10:57
X[1] = 0.3300 (0.0006) (0.0010)		
BLANK TEST	0.000	10:58

Average = 0.331
Std Dev = 0.0006

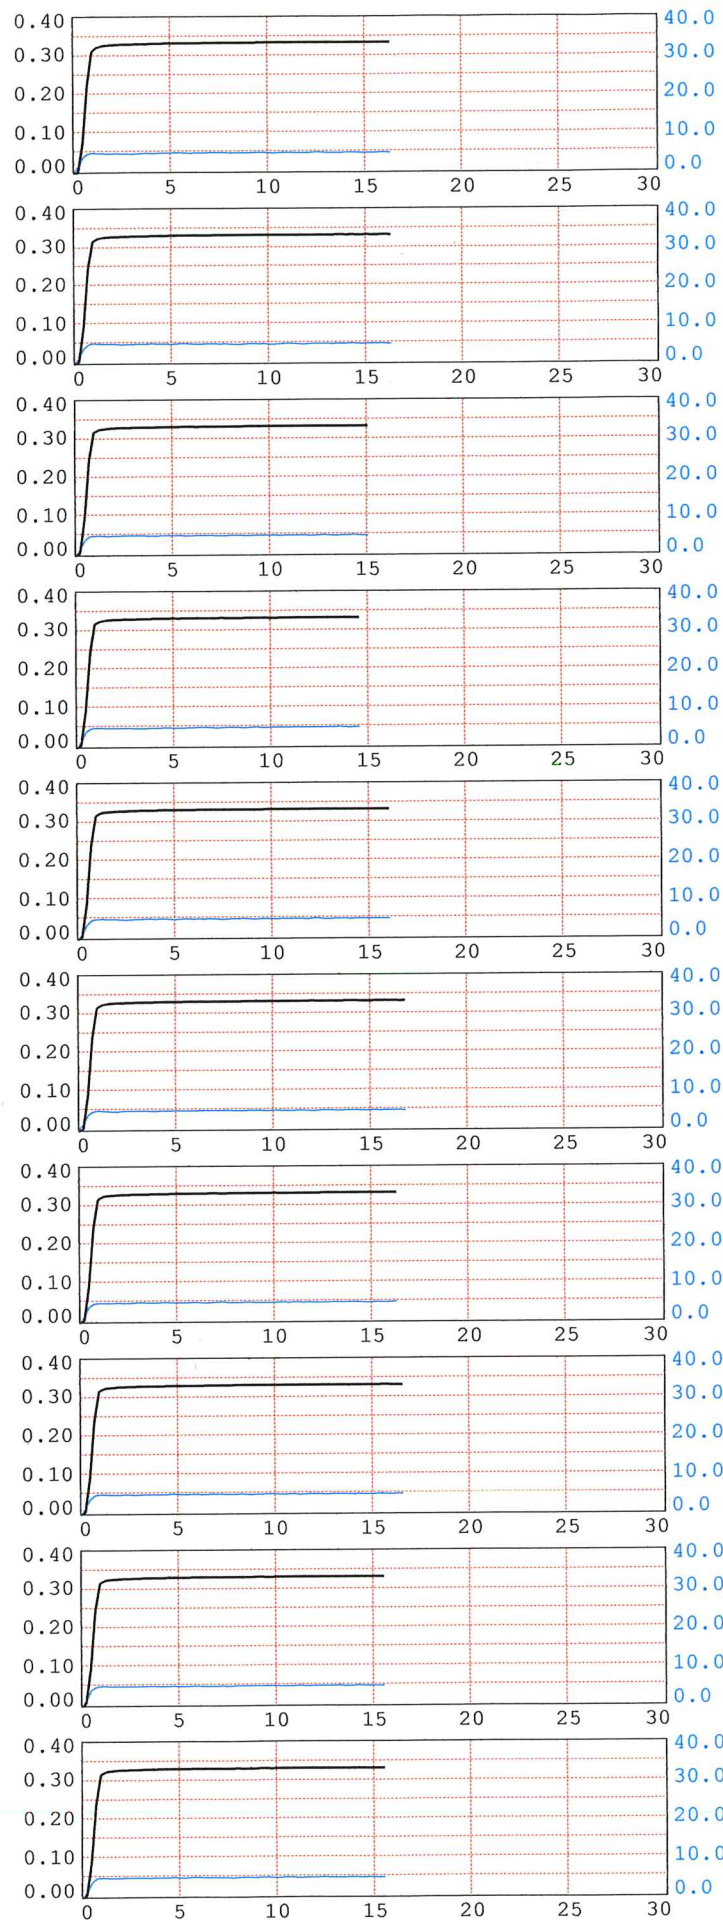

100146 *AS* 16