

INSTALLATION REPORT

DataMaster DMT: 100151
Location: Newport PD
Calibration Date: 10/07/2011
Certification Date: 10/12/2011
Installation Date: 10/25/2011
Installed by: STEVEN E HARNOIS



Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

VERSIONS

DMT: 1.00
PIC: 2.05
Modem: 2.1
Questions: 2.0

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube = 41.9°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.68 V
Cooler Voltage = 1.68 V
Bias Voltage = 80 V
Chopper Freq = 532 Hz

PUMP INFO

Flow Rate = 5.788 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.0305	0.0360
MIN (V)	0.0291	0.0348

FILTER INFO

Filter	Value	Zero
Filter 1	0.035	true
Filter 2	0.373	true
Filter 3	1.116	true

CALIBRATION CHECK

Xq = 0.084 0.51%

Accuracy and Precision Check


Concentration	= 0.102 g/210L
Lot #	= 12-13-100
Range	= 0.097 - 0.107
Average	= 0.099 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

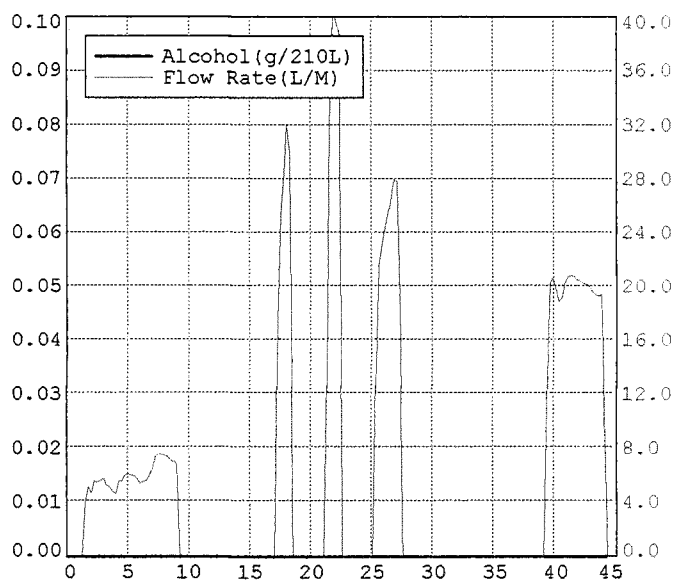

INSTALLATION PASSED

Performed by [Signature]

Date 10/25/2011

Reviewed by [Signature]

Date 10-25-11