

INSTALLATION REPORT

DataMaster DMT: 100151
Location: NEWPORT PD
Calibration Date: 10/07/2011
Certification Date: 10/12/2011
Installation Date: 02/16/2016
Installed by: ROBERT DRISCOLL



Default Options Loaded

Diagnostic Results

VERSIONS

DMT: 2.00
PIC: 2.05
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.9°C
Breath Tube = 43.7°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.68 V
Cooler Voltage = 1.69 V
Bias Voltage = 80 V
Chopper Freq = 533 Hz

PUMP INFO

Flow Rate = 5.790 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.2089	0.2140
MIN (V)	0.2075	0.2126

FILTER INFO

Filter	Value	Zero
Filter 1	0.213	true
Filter 2	0.542	true
Filter 3	1.251	true

CALIBRATION CHECK

Xq = 0.085 1.44%

INSTALLATION PASSED

Accuracy and Precision Check


Concentration	= 0.100 g/210L
Lot #	= 15-25-100
Range	= 0.095 - 0.105
Average	= 0.099 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

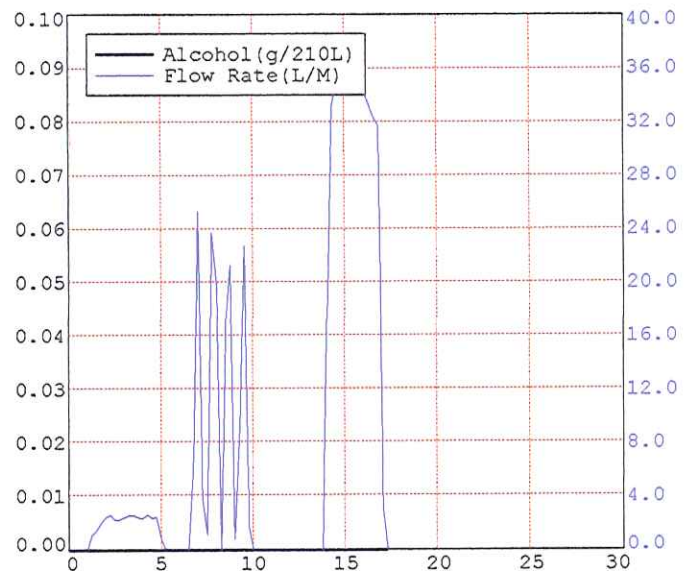

NIST Thermometer S/N 111814367 34.0°C
Moved into new processing room. RCD 2/16/16

Performed by

RCD

Date

02/16/2016

Reviewed by

[Signature]

Date

2/17/16

VERMONT FORENSIC LABORATORY

PO BOX 47
WATERBURY, VERMONT 05676-0047
TEL: 802-244-8788
FAX: 802-241-5557
<http://vfl.vermont.gov>



DataMaster DMT Site Evaluation Checklist

Agency or Site Information	
Name:	<u>Newport PD</u>
Address:	<u>222 Main Street</u> <u>Newport, VT 05855</u>
Phone:	<u>(802) 334-6733</u>
Fax:	<u>(802) 334-2818</u>

Personnel Information	
Head of Site:	<u>Chief Seth DiSanto</u>
Current DataMaster Supervisor (s):	<u>Charles Moulton</u>
Proposed DataMaster Supervisor(s):	

(Proposed) DataMaster DMT Environment		
Limited Controlled Access:	☒ Y	☐ N
Low Activity Area:	☒ Y	☐ N
Unlimited Access by Other Law Enforcement Personnel	☒ Y	☐ N
Access by VFL Technical Services	☒ Y	☐ N
Air Conditioned	☒ Y	☐ N
Room Temperature 65° - 85° F	☒ Y	☐ N
Adequate Ventilation	☒ Y	☐ N
Free of Cleaning Supplies	☒ Y	☐ N
Clean	☒ Y	☐ N

(Proposed) DataMaster DMT Connection(s)		
Power:		
Min 15 Amp	☒ Y	☐ N
Limited low power sharing:	☒ Y	☐ N
Ethernet Available:	☒ Y	☐ N
Distance to Ethernet	<u>2'</u>	

(Proposed) DataMaster DMT Site Maintenance Agreement		
Will notify VFL Alcohol Program staff of maintenance and supply needs promptly:	☒ Y	☐ N
Will notify VFL Alcohol Program staff of changes in building conditions or moves promptly:	☒ Y	☐ N
Will notify VFL Alcohol Program staff of relevant personnel changes at site promptly:	☒ Y	☐ N

VFL Representative:	<u>Robert Driscoll</u>	<u>[Signature]</u>	<u>2/16/16</u>
	Print Name	Signature	Date
Agency Representative:	<u>Seth DiSanto</u>	<u>[Signature]</u>	<u>2/16/16</u>
	Print Name	Signature	Date

100151

2nd 2 KID