

INSTALLATION REPORT

DataMaster DMT: 100151
Location: NEWPORT PD
Calibration Date: 04/25/2017
Certification Date: 04/25/2017
Installation Date: 04/26/2017
Installed by: ROBERT DRISCOLL



Default Options Loaded

Diagnostic Results

VERSIONS
DMT: 2.03
PIC: 2.05
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.6°C
Breath Tube = 42.4°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.73 V
Cooler Voltage = 1.71 V
Bias Voltage = 80 V
Chopper Freq = 527 Hz

PUMP INFO

Flow Rate = 4.691 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.0348	0.0402
MIN (V)	0.0335	0.0390

FILTER INFO

Filter	Value	Zero
Filter 1	0.040	true
Filter 2	0.379	true
Filter 3	1.100	true

CALIBRATION CHECK

Xq = 0.086 0.00%

INSTALLATION PASSED

Accuracy and Precision Check


Concentration	= 0.101 g/210L
Lot #	= 17-16-100
Range	= 0.096 - 0.106
Average	= 0.100 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

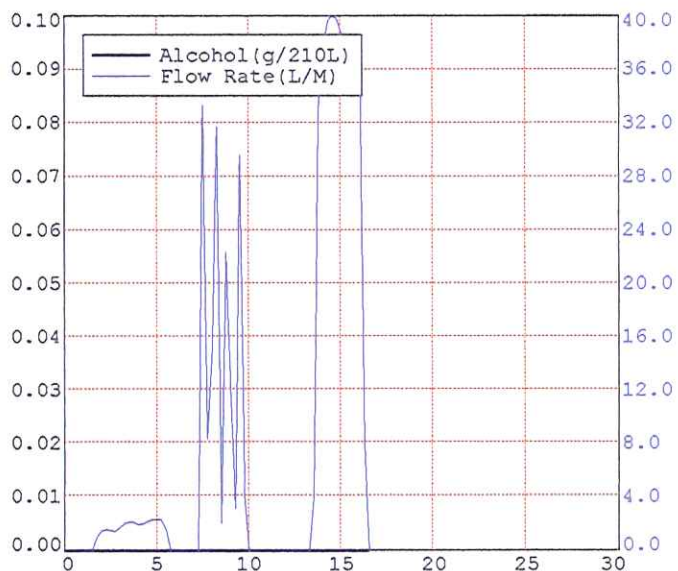

Performed by

RD

Date

04/26/2017

Reviewed by

AB

Date

4/28/17