

ROUTINE PERFORMANCE CHECK REPORT



DataMaster DMT: 100151
Location: NEWPORT PD
Calibration Date: 04/25/2017
Certification Date: 04/25/2017
Installation Date: 04/26/2017
RPC Date: 02/15/2019
Supervisor Name: CHARLES D MOULTON

Diagnostic Results

VERSIONS
DMT: 2.05
PIC: 2.08
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.9°C
Breath Tube = 44.3°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.73 V
Cooler Voltage = 1.71 V
Bias Voltage = 80 V
Chopper Freq = 542 Hz

PUMP INFO

Flow Rate = 4.905 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	0.4449	0.4488
MIN(V)	0.4435	0.4474

FILTER INFO

Filter	Value	Zero
Filter 1	0.448	true
Filter 2	0.759	true
Filter 3	1.442	true

CALIBRATION CHECK

Xq = 0.088 1.71%

Routine Performance Check Passed

Accuracy and Precision Check


Concentration	= 0.101 g/210L
Lot #	= 18-19-100
Range	= 0.096 - 0.106
Average	= 0.100 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

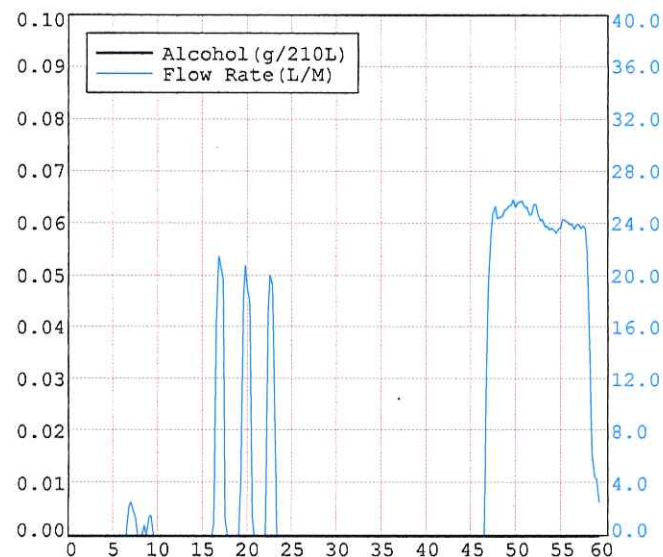

Performed by

[Signature]

Date

02/15/2019

Reviewed by

[Signature]

Date

2/18/19

[Signature]
2/25/19

DMT Serial Number #100151

Page 1 of 1

02/15/2019 8:21 PM