

ROUTINE PERFORMANCE CHECK REPORT



DataMaster DMT: 100151
Location: NEWPORT PD
Calibration Date: 04/25/2017
Certification Date: 04/25/2017
Installation Date: 04/26/2017
RPC Date: 06/29/2019
Supervisor Name: CHARLES D MOULTON

Diagnostic Results

VERSIONS
DMT: 2.05
PIC: 2.08
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.8°C
Breath Tube = 47.1°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.73 V
Cooler Voltage = 1.71 V
Bias Voltage = 80 V
Chopper Freq = 541 Hz

PUMP INFO

Flow Rate = 4.854 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	0.6299	0.6323
MIN(V)	0.6283	0.6313

FILTER INFO

Filter	Value	Zero
Filter 1	0.632	true
Filter 2	0.932	true
Filter 3	1.600	true

CALIBRATION CHECK

Xq = 0.088 1.41%

Routine Performance Check Passed

Accuracy and Precision Check


Concentration = 0.101 g/210L
Lot # = 18-19-100
Range = 0.096 - 0.106
Average = 0.101 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

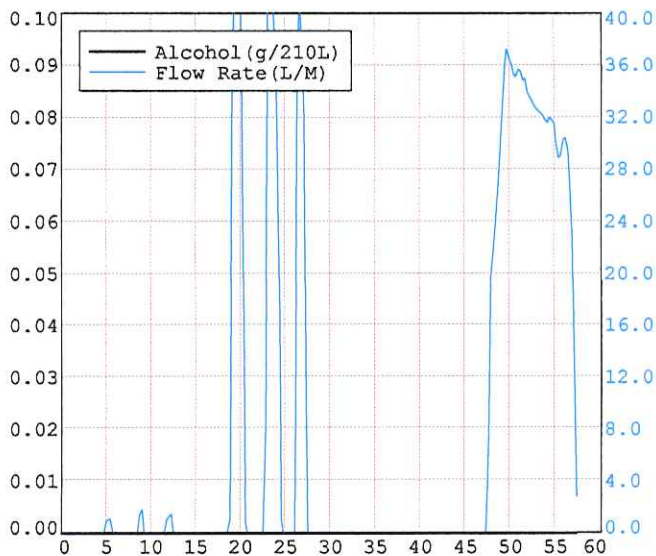

Performed by

Date

06/29/2019

Reviewed by

Date

7/1/2019

DMT Serial Number #100151

Page 1 of 1

06/29/2019 1:16 AM