

INSTALLATION REPORT

DataMaster DMT: 100151
Location: NEWPORT PD
Calibration Date: 03/31/2021
Certification Date: 03/31/2021
Installation Date: 04/09/2021
Installed by: SARAH STRATTON



Default Options Loaded

Diagnostic Results

VERSIONS
DMT: 2.06
PIC: 3.07
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube = 43.1°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.84 V
Cooler Voltage = 1.83 V
Bias Voltage = 80 V
Chopper Freq = 526 Hz

PUMP INFO

Flow Rate = 4.924 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	0.0213	0.0268
MIN(V)	0.0197	0.0250

FILTER INFO

Filter	Value	Zero
Filter 1	0.026	true
Filter 2	0.360	true
Filter 3	1.114	true

CALIBRATION CHECK

Xq = 0.088 0.00%

INSTALLATION PASSED

Accuracy and Precision Check


Concentration	= 0.100 g/210L
Lot #	= 21-05-100
Range	= 0.095 - 0.105
Average	= 0.097 g/210L
Std Dev	= 0.0005

RF Detection Test

Passed
RF detected

Sample Acceptance Test

Passed

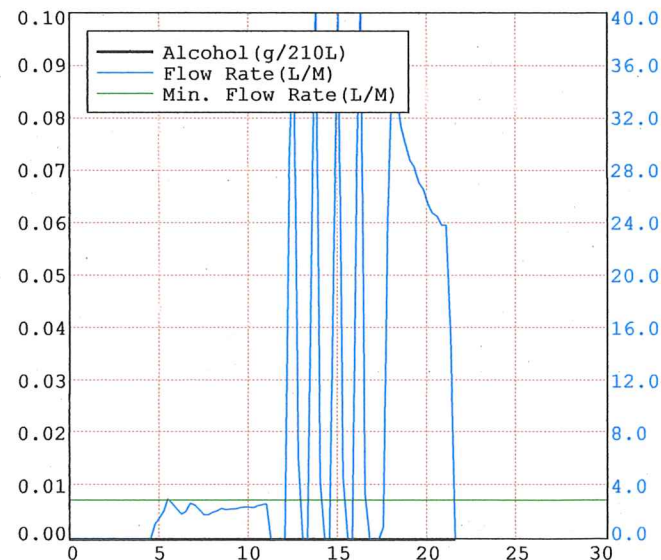

Performed by

SJS SJS

Date

04/09/2021

Reviewed by

[Signature]

Date

4/13/21

DMT Serial Number #100151

Page 1 of 1

04/09/2021 11:17 AM