

ROUTINE PERFORMANCE CHECK REPORT



DataMaster DMT: 100151
Location: NEWPORT PD
Calibration Date: 03/31/2021
Certification Date: 03/31/2021
Installation Date: 04/09/2021
RPC Date: 06/30/2021
Supervisor Name: CHARLES D MOULTON

Diagnostic Results

VERSIONS

DMT: 2.06
PIC: 3.07
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube = 48.1°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.84 V
Cooler Voltage = 1.83 V
Bias Voltage = 80 V
Chopper Freq = 534 Hz

PUMP INFO

Flow Rate = 4.749 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	0.0130	0.0154
MIN(V)	0.0116	0.0140

FILTER INFO

Filter	Value	Zero
Filter 1	0.015	true
Filter 2	0.355	true
Filter 3	1.149	true

CALIBRATION CHECK

Xq = 0.088 0.20%

Routine Performance Check Passed

Accuracy and Precision Check


Concentration = 0.100 g/210L
Lot # = 21-05-100
Range = 0.095 - 0.105
Average = 0.098 g/210L
Std Dev = 0.0000

RF Detection Test

Passed
RF detected

Sample Acceptance Test

Passed

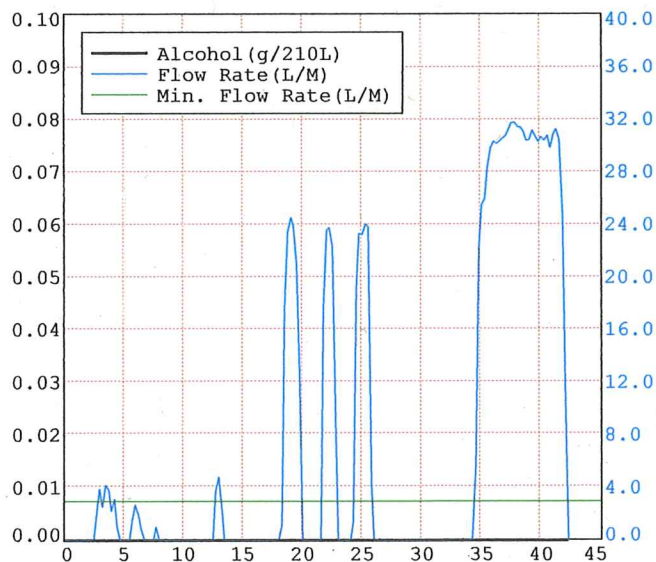

Performed by

CA [signature]

Date

06/30/2021

Reviewed by

SJS

Date

7/1/2021

[Signature]
7/1/21