

ROUTINE PERFORMANCE CHECK REPORT



DataMaster DMT: 100151
Location: NEWPORT PD
Calibration Date: 03/31/2021
Certification Date: 03/31/2021
Installation Date: 04/09/2021
RPC Date: 10/27/2023
Supervisor Name: CHARLES D MOULTON

Diagnostic Results

VERSIONS
DMT: 2.06
PIC: 3.07
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.8°C
Breath Tube = 45.1°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.84 V
Cooler Voltage = 1.83 V
Bias Voltage = 80 V
Chopper Freq = 536 Hz

PUMP INFO

Flow Rate = 4.681 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.0470	0.0502
MIN (V)	0.0437	0.0490

FILTER INFO

Filter	Value	Zero
Filter 1	0.050	true
Filter 2	0.405	true
Filter 3	1.146	true

CALIBRATION CHECK

Xq = 0.089 1.48%

Routine Performance Check Passed

Accuracy and Precision Check


Concentration = 0.101 g/210L
Lot # = 23-02-100
Range = 0.096 - 0.106
Average = 0.098 g/210L
Std Dev = 0.0000

RF Detection Test

Passed
RF detected

Sample Acceptance Test

Passed

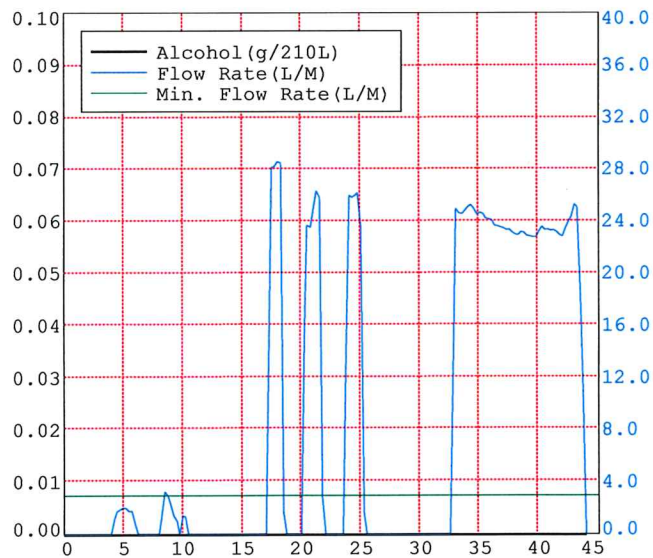

Performed by

[Signature]

Date

10/27/2023

Reviewed by

[Signature]

Date

10/30/23

[Signature]
11/3/23

DMT Serial Number #100151

Page 1 of 1

10/27/2023 8:29 PM