

INSTALLATION REPORT

DataMaster DMT: 100156
Location: Fair Haven PD
Calibration Date: 12/24/2012
Certification Date: 12/24/2012
Installation Date: 12/26/2012
Installed by: ROBERT DRISCOLL



Default Options Loaded

Diagnostic Results

VERSIONS

DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.9°C
Breath Tube = 47.9°C
Digital Sim = 34.1°C

SETTINGS

Lamp Voltage = 1.85 V
Cooler Voltage = 1.82 V
Bias Voltage = 80 V
Chopper Freq = 546 Hz

PUMP INFO

Flow Rate = 5.883 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.3234	0.3274
MIN (V)	0.3220	0.3254

FILTER INFO

Filter	Value	Zero
Filter 1	0.326	true
Filter 2	0.450	true
Filter 3	1.350	true

CALIBRATION CHECK

Xq = 0.084 0.51%

Accuracy and Precision Check


Concentration	= 0.099 g/210L
Lot #	= 12-77-100
Range	= 0.094 - 0.104
Average	= 0.101 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

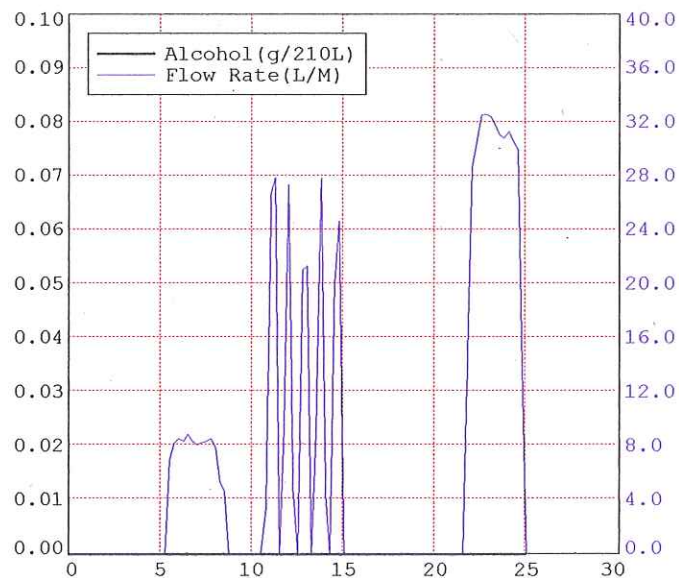

INSTALLATION PASSED

Performed by

[Signature]

Date

12/26/2012

Reviewed by

[Signature]

Date

12/31/2012