

INSTALLATION REPORT

DataMaster DMT: 100156
Location: FAIR HAVEN PD / RUTLAND VSP
Calibration Date: 02/22/2016
Certification Date: 02/22/2016
Installation Date: 02/23/2016
Installed by: ROBERT DRISCOLL



Default Options Loaded

Diagnostic Results

VERSIONS
DMT: 2.00
PIC: 2.05
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube = 45.3°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.64 V
Cooler Voltage = 1.69 V
Bias Voltage = 80 V
Chopper Freq = 538 Hz

PUMP INFO

Flow Rate = 6.090 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.0543	0.0594
MIN (V)	0.0528	0.0579

FILTER INFO

Filter	Value	Zero
Filter 1	0.058	Zero = true
Filter 2	0.337	Zero = true
Filter 3	1.013	Zero = true

CALIBRATION CHECK

Xq = 0.098 0.80%

INSTALLATION PASSED

Accuracy and Precision Check


Concentration = 0.099 g/210L
Lot # = 15-13-100
Range = 0.094 - 0.104
Average = 0.101 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

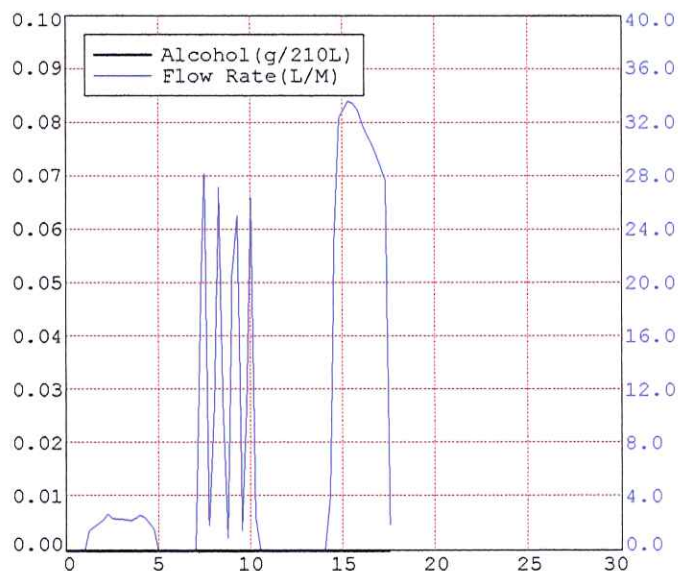

NIST Thermometer s/n 111814367 34.1°C

RCD
2/23/16

Performed by

AB RCD

Date

02/23/2016

Reviewed by

AB

Date

2/26/16