

INSTALLATION REPORT

DataMaster DMT: 100156
Location: FAIR HAVEN PD
Calibration Date: 03/10/2017
Certification Date: 03/10/2017
Installation Date: 03/13/2017
Installed by: ROBERT DRISCOLL



Default Options Loaded

Diagnostic Results

VERSIONS
DMT: 2.03
PIC: 2.05
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube = 44.0°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.64 V
Cooler Voltage = 1.71 V
Bias Voltage = 80 V
Chopper Freq = 525 Hz

PUMP INFO

Flow Rate = 5.343 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	-0.0384	-0.0317
MIN (V)	-0.0398	-0.0335

FILTER INFO

Filter 1	-0.033	Zero = true
Filter 2	0.251	Zero = true
Filter 3	0.919	Zero = true

CALIBRATION CHECK

Xq = 0.097 0.71%

INSTALLATION PASSED

Accuracy and Precision Check


Concentration	= 0.101 g/210L
Lot #	= 17-10-100
Range	= 0.096 - 0.106
Average	= 0.098 g/210L
Std Dev	= 0.0005

RF Detection Test

Passed

Sample Acceptance Test

Passed

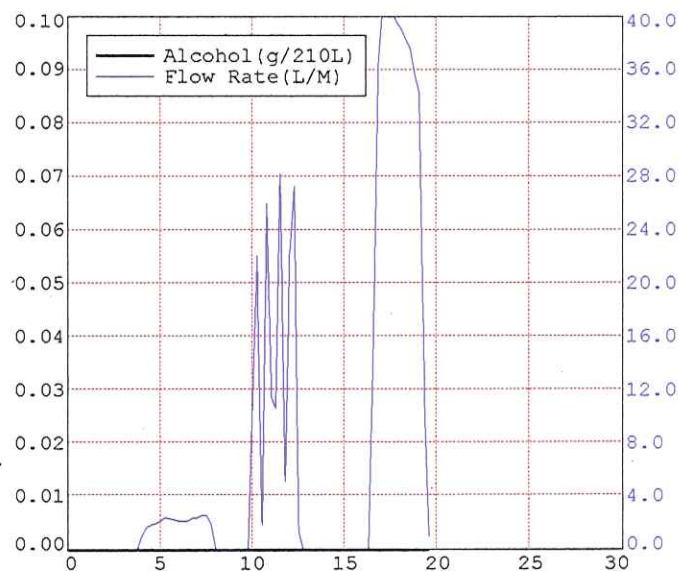

Performed by

RD

Date

03/13/2017

Reviewed by

AB

Date

3/16/17