

Start Date 3/10/17

DMT Serial # 100156

DMT Location Fair Haven PD

DMT Upgrade Checklist

	Initials	Date
• Install new Property Identification Tag Tag# <u>1000915</u>	<u>RCD</u>	<u>3/10/17</u>
• Download Data	<u>RCD</u>	<u>3/10/17</u>
• Upload New Software	<u>RCD</u>	<u>3/10/17</u>
• Install Intoximeters 12V500 conversion kit	<u>RCD</u>	<u>3/10/17</u>
• Performance check a new Guth 12V500 simulator using temp check form Sticker applied to sim? ☒	<u>RCD</u>	<u>3/10/17</u>
• Install new Guth 12V500 12V500 s/n: <u>MP3474</u>	<u>RCD</u>	<u>3/10/17</u>
• Verify adjustable flow rate valve installed (If no, install and set volume to 1.5L)	<u>RCD</u>	<u>3/10/17</u>
• Perform Calibration Protocol	<u>RCD</u>	<u>3/10/17</u>
• Perform Certification Protocol	<u>RCD</u>	<u>3/10/17</u>
• Calibration and certification review by analyst	<u>JSD</u>	<u>3/13/17</u>
• Data logged into control charts	<u>JSD</u>	<u>3/13/17</u>

Reviewed by: [Signature] Date: 3/13/2017

CALIBRATION REPORT

DataMaster DMT: 100156
Calibration Date: 03/10/2017
Calibrated by: ROBERT DRISCOLL
Lot: 16-28-100



Ca	=	0.100		
CAL	=	0.958145	0.800	<= CAL < 1.200
b1	=	0.000	0.000	<= b1 < 0.004
b2	=	0.005	0.002	<= b2 < 0.010
b3	=	0.000	0.000	<= b3 < 0.004
Xq	=	0.098	0.050	<= Xq < 0.200
a21	=	1.193609	1.050	<= a21 < 1.300
a31	=	0.454092	0.300	<= a31 < 0.800

BL-DMT11152016 RCD 3/10/17

Performed by

RCD

Date

03/10/2017



ACCURACY & PRECISION REPORT

STATE OF VERMONT

DataMaster DMT: 100156

Date: 03/10/2017

Time: 09:15:46

SUPERVISOR NAME:

RCD CAL CHECK


SOLUTION LOT #: GUTH 16160

SOLUTION CONCENTRATION: 0.098

BLANK TEST	0.000	09:16
CALIBRATION CHECK	PASSED	09:16
SIMULATOR VAPOR 34.0°C	0.097	09:17
SIMULATOR VAPOR 34.0°C	0.096	09:18
SIMULATOR VAPOR 34.0°C	0.096	09:19
SIMULATOR VAPOR 34.0°C	0.096	09:20
SIMULATOR VAPOR 34.0°C	0.096	09:21
SIMULATOR VAPOR 34.0°C	0.096	09:22
SIMULATOR VAPOR 34.0°C	0.097	09:23
SIMULATOR VAPOR 34.0°C	0.096	09:24
SIMULATOR VAPOR 34.0°C	0.096	09:25
SIMULATOR VAPOR 34.0°C	0.096	09:26
BLANK TEST	0.000	09:27

Average = 0.096

Std Dev = 0.0004

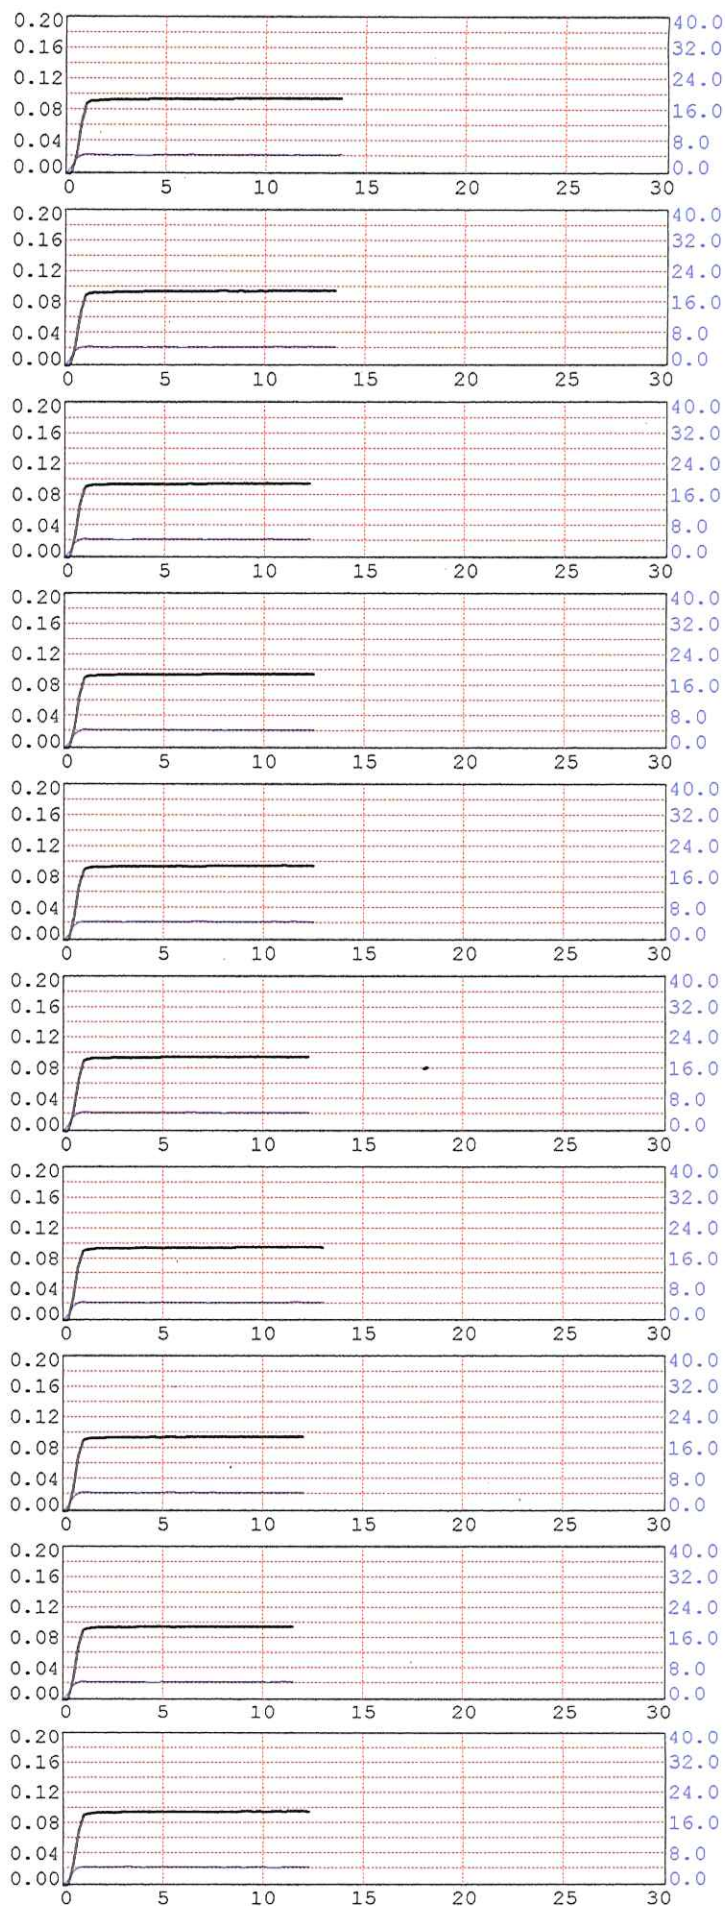

3

850

CERTIFICATION REPORT

DataMaster DMT: 100156
Calibration Date: 03/10/2017
Certification Date: 03/10/2017
Certified by: ROBERT DRISCOLL



Diagnostic Results

VERSIONS

DMT: 2.03
PIC: 2.05
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube = 45.3°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.64 V
Cooler Voltage = 1.71 V
Bias Voltage = 80 V
Chopper Freq = 533 Hz

PUMP INFO

Flow Rate = 5.201 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.0465	0.0508
MIN (V)	0.0451	0.0494

FILTER INFO

Filter 1	0.050	Zero = true
Filter 2	0.330	Zero = true
Filter 3	1.032	Zero = true

CALIBRATION CHECK

Xq = 0.098 0.36%

Options

OPTIONS

Units

Alcohol..... g/210L

Simulator

Tolerance Check..... yes
Standard Type..... wet
Nominal..... 0.100
Digital Simulator..... Guth

Subject

Ask Questions..... yes
Number of Tests..... 2
Alcohol Display..... yes
Volume Display..... yes
Query Refusal..... yes
Copies..... 3
Simulator Before..... yes
Simulator Between..... yes
Simulator After..... no
Observation Time..... 0

Supervisor

Number of Tests..... 10

Calibration

Standard Type..... wet
Nominal..... 0.100
Nominal (Dry Gas)..... 0.100
Number of Tests..... 1

Printer

Printer On..... yes

Software Configuration

Data Collection..... yes

Linearity Check Results

True Value	Reported Average	Std Dev
0.020 g/210L	0.019 g/210L	0.0000
Lot # 16-24-020		
0.080 g/210L	0.078 g/210L	0.0000
Lot # 16-38-080		
0.164 g/210L	0.156 g/210L	0.0005
Lot # 16-26-160		
0.372 g/210L	0.355 g/210L	0.0005
Lot # 16-40-360		

$R^2 = 1$

Acetone Interference Test

Lot # 17-11-08A2

Interference Detected

Mouth Alcohol Test

Mouth Alcohol Detected




RF Detection Test

Passed

Sample Acceptance Test

Passed

CERTIFICATION PASSED

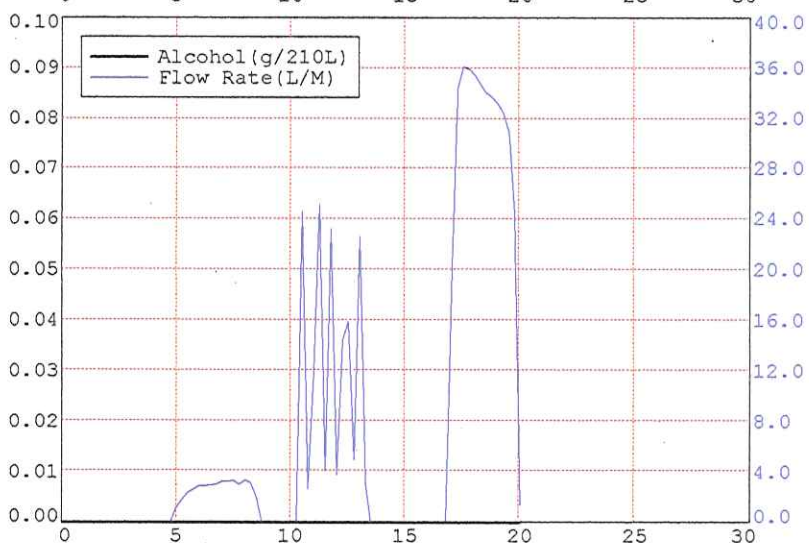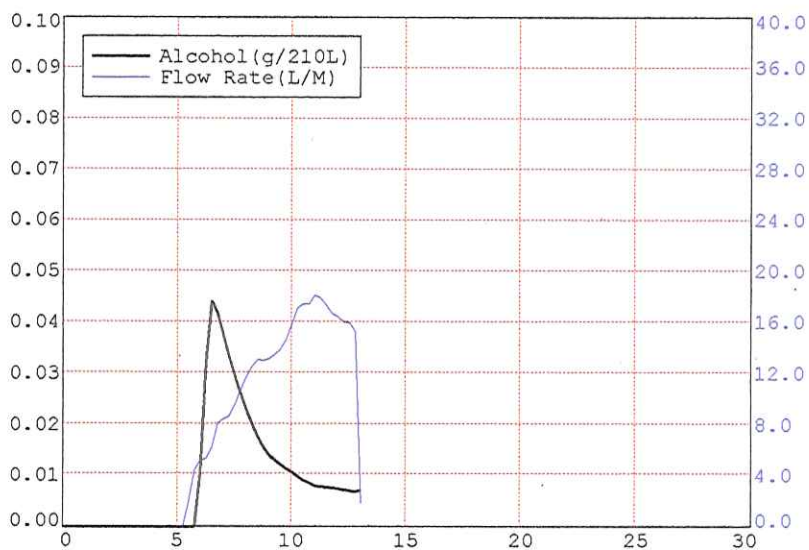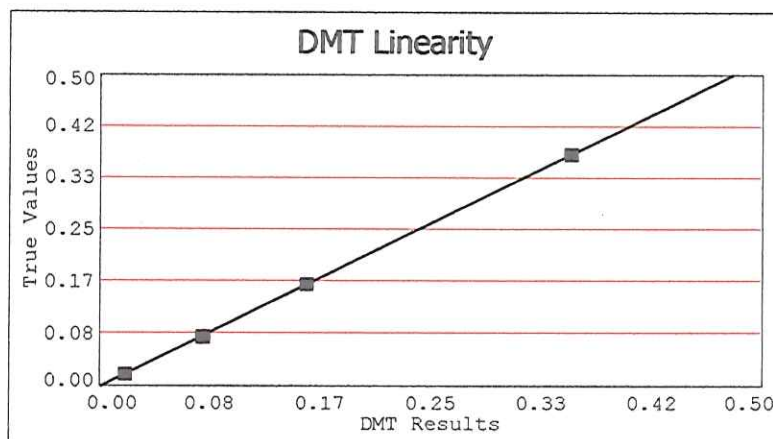

Performed by

726 RCD

Date

03/10/2017

Reviewed by

[Signature]

Date

3/13/17

DMT Serial Number #100156

Page 2 of 2

03/10/2017 10:44 AM

5

150