

INSTALLATION REPORT

DataMaster DMT: 100157
Location: Colchester PD
Calibration Date: 02/07/2012
Certification Date: 02/08/2012
Installation Date: 02/17/2012
Installed by: STEVEN E HARNOIS



Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.2
Questions: 2.0

TEMPERATURES

Sample Chamber = 49.1°C
Breath Tube = 43.2°C
Digital Sim = 34.1°C

SETTINGS

Lamp Voltage = 1.63 V
Cooler Voltage = 1.67 V
Bias Voltage = 80 V
Chopper Freq = 540 Hz

PUMP INFO

Flow Rate = 5.557 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	-0.1870	-0.1827
MIN (V)	-0.1886	-0.1841

FILTER INFO

Filter	Value	Zero
Filter 1	-0.184	true
Filter 2	0.127	true
Filter 3	1.259	true

CALIBRATION CHECK

Xq = 0.094 0.55%

Accuracy and Precision Check


Concentration	= 0.100 g/210L
Lot #	= 12-58-100
Range	= 0.095 - 0.105
Average	= 0.100 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

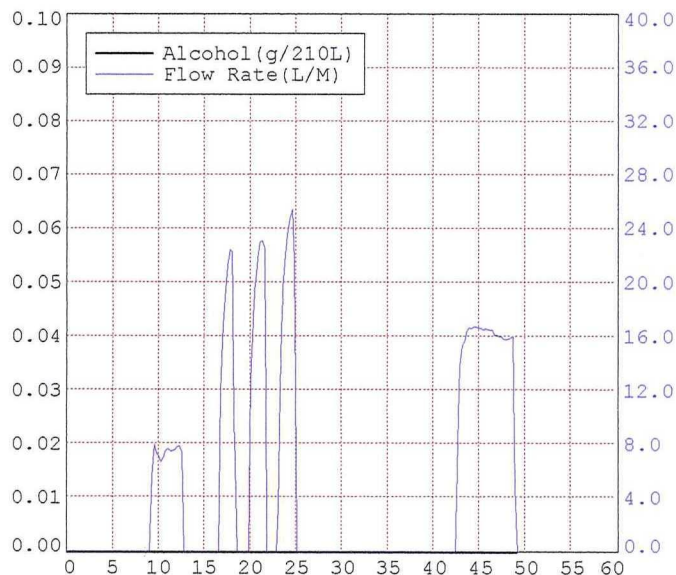

INSTALLATION PASSED

Performed by

Date 02/17/2012

Reviewed by

Date 2/17/12

Rev.
KMK
2-18-12

INSTALLATION REPORT

DataMaster DMT: 100157
Location: Colchester PD
Calibration Date: 02/07/2012
Certification Date: 02/08/2012
Installation Date: 02/17/2012
Installed by: STEVEN E HARNOIS



Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.2
Questions: 2.0

TEMPERATURES

Sample Chamber = 49.0°C
Breath Tube = 44.9°C
Digital Sim = 34.2°C

SETTINGS

Lamp Voltage = 1.63 V
Cooler Voltage = 1.67 V
Bias Voltage = 80 V
Chopper Freq = 537 Hz

PUMP INFO

Flow Rate = 5.520 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	-0.1933	-0.1884
MIN (V)	-0.1949	-0.1896

FILTER INFO

Filter	Value	Zero
Filter 1	-0.189	true
Filter 2	0.122	true
Filter 3	1.239	true

CALIBRATION CHECK

Xq = 0.094 0.92%


Accuracy and Precision Check

Concentration	= 0.100 g/210L
Lot #	= 12-58-100
Range	= 0.095 - 0.105
Average	= 0.099 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

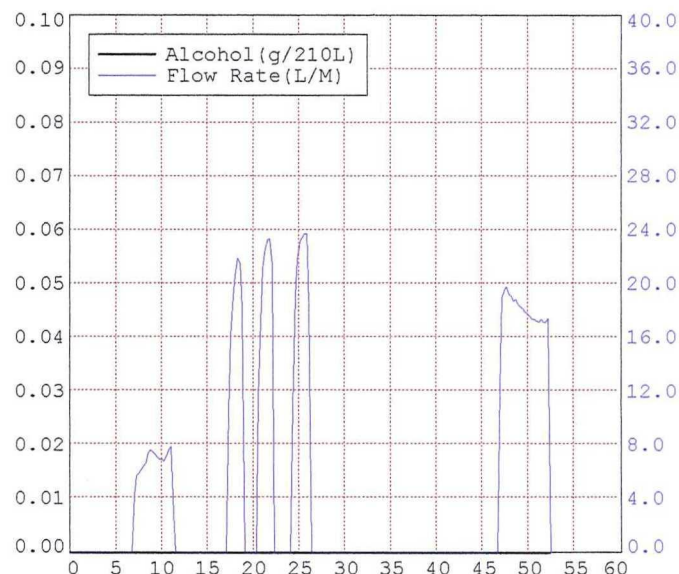

INSTALLATION FAILED

Blank error after sample acceptance test. (1) 2/17/12

Performed by STEVEN E HARNOIS

Date 02/17/2012

Reviewed by _____

Date _____