

ROUTINE PERFORMANCE CHECK REPORT



DataMaster DMT: 100157
Location: Colchester PD
Calibration Date: 02/07/2012
Certification Date: 02/08/2012
Installation Date: 09/12/2012
RPC Date: 01/20/2014
Supervisor Name: JACK B LEHNEMAN

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.8°C
Breath Tube = 44.1°C
Digital Sim = 34.2°C

SETTINGS

Lamp Voltage = 1.63 V
Cooler Voltage = 1.67 V
Bias Voltage = 80 V
Chopper Freq = 553 Hz

PUMP INFO

Flow Rate = 5.406 L/M

DETECTOR INFO

PUMP ON OFF
MAX (V) -0.0878 -0.0844
MIN (V) -0.0896 -0.0858

FILTER INFO

Filter 1 -0.086 Zero = true
Filter 2 0.221 Zero = true
Filter 3 1.342 Zero = true

CALIBRATION CHECK

Xq = 0.094 0.55%

Routine Performance Check Passed

Accuracy and Precision Check


Concentration = 0.099 g/210L
Lot # = 13-19-100
Range = 0.094 - 0.104
Average = 0.099 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

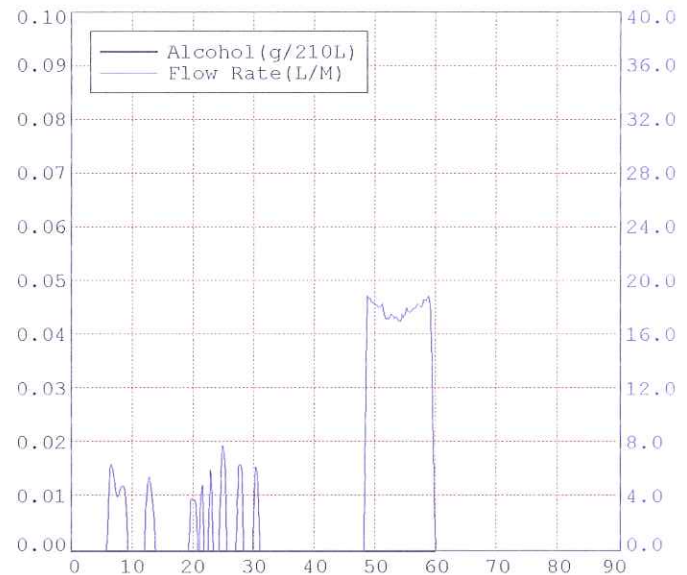

Performed by

Jack B. Lehman

Date

01/20/2014

Reviewed by

[Signature]

Date

1/21/14

DMT Serial Number #100157

Page 1 of 1

01/20/2014 4:50 PM

[Signature]
1/22/2014