

ROUTINE PERFORMANCE CHECK REPORT



DataMaster DMT: 100157
Location: Colchester PD
Calibration Date: 02/07/2012
Certification Date: 02/08/2012
Installation Date: 09/12/2012
RPC Date: 06/19/2014
Supervisor Name: CHRISTOPHER M JONES

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.6°C
Breath Tube = 45.0°C
Digital Sim = 34.2°C

SETTINGS

Lamp Voltage = 1.63 V
Cooler Voltage = 1.67 V
Bias Voltage = 80 V
Chopper Freq = 553 Hz

PUMP INFO

Flow Rate = 5.511 L/M

DETECTOR INFO

PUMP ON OFF
MAX(V) -0.0409 -0.0374
MIN(V) -0.0427 -0.0390

FILTER INFO

Filter 1 -0.039 Zero = true
Filter 2 0.269 Zero = true
Filter 3 1.376 Zero = true

CALIBRATION CHECK

Xq = 0.094 0.65%

Accuracy and Precision Check


Concentration = 0.099 g/210L
Lot # = 13-21-100
Range = 0.094 - 0.104
Average = 0.097 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

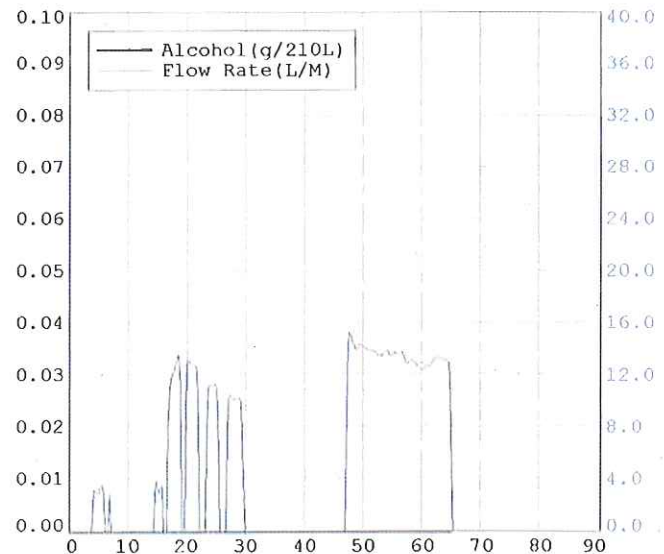

Routine Performance Check Passed

Performed by

C Jones M161

Date

06/19/2014

Reviewed by

[Signature]

Date

6/23/14

DMT Serial Number #100157

Page 1 of 1

06/19/2014 4:12 PM

[Signature]
6/23/2014