

Datamaster Monthly Update Checklist

Department/Agency: Wolchester P.D. DM serial #: 100157

Date: 3/1/2017 for month of February 2017

	Provided	None this month
Operators Logbook	<input checked="" type="checkbox"/>	<input type="checkbox"/>
Maintenance Logbook	<input checked="" type="checkbox"/>	<input type="checkbox"/>
Breath Summary Report	<input checked="" type="checkbox"/>	<input type="checkbox"/>
Status Summary Report	<input checked="" type="checkbox"/>	<input type="checkbox"/>
Calibration	<input type="checkbox"/>	<input type="checkbox"/>
Certification	<input type="checkbox"/>	<input type="checkbox"/>
Installation	<input type="checkbox"/>	<input type="checkbox"/>
Annual Preventative Maintenance	<input type="checkbox"/>	<input type="checkbox"/>
<hr/>		
Routine Performance Check	<input checked="" type="checkbox"/>	<input type="checkbox"/>
Simulator Solution Change	<input checked="" type="checkbox"/>	<input type="checkbox"/>
Other Reports	<input type="checkbox"/>	<input type="checkbox"/>

List other report type and date:

DETAILED RESULTS SUMMARY

03/01/2017

Test Date	Test Time	Agency	Operator Name	Alcohol Val. 1	Alcohol Val. 2	Sim. Conc. 1	Sim. Conc. 2	Status Message
02/01/2017	16:31:05	COLCHESTER PD	VICTOR BITCA	REFUSED		0.093		
02/05/2017	23:21:35	COLCHESTER PD	CHRISTOPHER M JONES	0.169		0.095		
02/06/2017	01:44:55	COLCHESTER PD	CHRISTOPHER M JONES	0.122		0.095		
02/23/2017	03:20:40	COLCHESTER PD	STEPHEN J GUTIERREZ			0.091		Simulator Out of Range
02/23/2017	03:33:21	COLCHESTER PD	STEPHEN J GUTIERREZ			0.091		Simulator Out of Range
02/24/2017	21:25:31	COLCHESTER PD	VICTOR BITCA	0.116	0.105	0.098	0.096	

DATAMASTER DMT OPERATOR USE LOG

Colchester PD
Department/Agency

100157
DataMaster DMT Serial Number

Date	DMT Operator's Name	Subject's Name	Simulator Vapor 1	Simulator Vapor 2
10/30/16	J. TRETER	TANYA SNYDER		
11-1-16	C Jones	Shane Gallo	.096	.096
11/3/16	S. GUTIERREZ	DEBORAH MOCUSKER	.096	
11/13/16	J. TRETER	TASHA MANCHESTER	.096	.094
11/13/16	S. GUTIERREZ	MELISSA CARACANON	.096	.095
11/30/16	V. BITCA	Melissa Bouchard	.095	
12/02/16	M. AKERLIND	JANAK GURUNG	.095	
12-08-16	West	Charles Cota	.095	
12-20-16	V. BITCA	Samuel Bombard	.094	
01-06-17	West	Matthew Yehent	.094	.093
01-19-17	Jones	Sol. Change	.098	
01/22/17	Fontana	Scott Mercure	.096	.094
1/29/17	R. CURRIER	JESSE ZIGES		
2/1/17	V. BITCA	Robert Lopez	.093	
2-5-17	C Jones	Charles Nahn	.098	
2-6-17	C Jones	Gary Pasquale	.095	
2/23/17	S. GUTIERREZ	C. MONECCI	.098	
2/24/17	C Jones	Solution Change RPC	.097	
2/24/17	V. BITCA	Thomas Slimm	.098	.096

DATAMASTER DMT MAINTENANCE LOG

Colchester Police
Department/Agency

DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
2/24/17	<p>DMT External Standard Solution Lot # 16-21-100 EtOHaq Conc: 0.098 Range: 0.093 - 0.103 Preparation Date: 9/13/2016 Expires: 9/13/2017 OPENED: 2-24-17 CMS</p> <p>[For RP ice Label Here]</p> <p>RPC / Solution Change</p>	<p>CMS MIS</p>
	<p>[For RPC or Simulator Solution Change Place Label Here]</p>	
	<p>[For RPC or Simulator Solution Change Place Label Here]</p>	
	<p>[For RPC or Simulator Solution Change Place Label Here]</p>	
	<p>[For RPC or Simulator Solution Change Place Label Here]</p>	

ROUTINE PERFORMANCE CHECK REPORT



DataMaster DMT: 100157
Location: Colchester PD
Calibration Date: 02/07/2012
Certification Date: 02/08/2012
Installation Date: 09/12/2012
RPC Date: 02/24/2017
Supervisor Name: CHRISTOPHER M JONES

Diagnostic Results

VERSIONS
DMT: 2.00
PIC: 2.05
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.9°C
Breath Tube = 45.9°C
Digital Sim = 34.1°C

SETTINGS

Lamp Voltage = 1.63 V
Cooler Voltage = 1.67 V
Bias Voltage = 80 V
Chopper Freq = 555 Hz

PUMP INFO

Flow Rate = 4.423 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.1750	0.1781
MIN (V)	0.1732	0.1764

FILTER INFO

Filter 1	0.177	Zero = true
Filter 2	0.471	Zero = true
Filter 3	1.537	Zero = true

CALIBRATION CHECK

Xq = 0.094 0.18%

Routine Performance Check Passed

Accuracy and Precision Check


Concentration = 0.098 g/210L
Lot # = 16-21-100
Range = 0.093 - 0.103
Average = 0.097 g/210L
Std Dev = 0.0008

RF Detection Test

Passed

Sample Acceptance Test

Passed

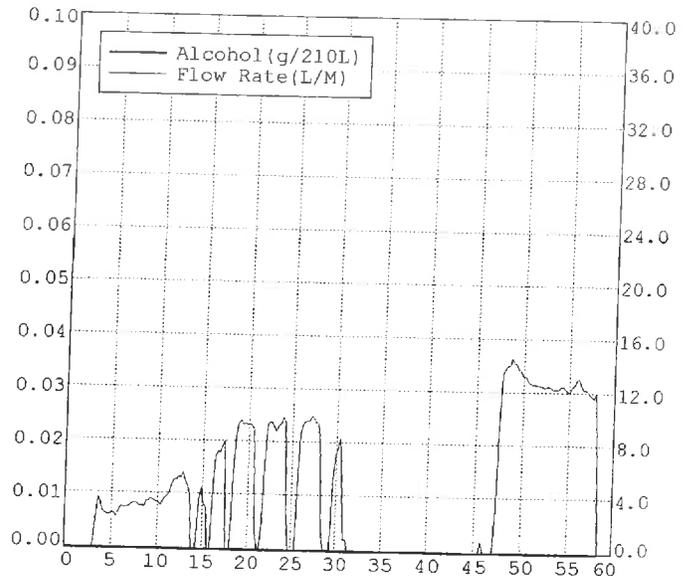

Performed by

Chris M151


Date

02/24/2017

Reviewed by

Date

ROUTINE PERFORMANCE CHECK REPORT

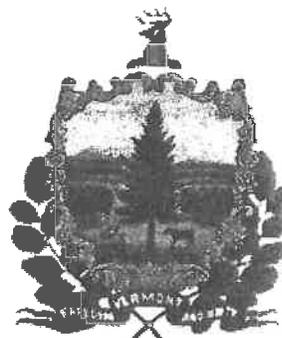

DataMaster DMT: 100157
Location: Colchester PD
Calibration Date: 02/07/2012
Certification Date: 02/08/2012
Installation Date: 09/12/2012
RPC Date: 02/24/2017
Supervisor Name: CHRISTOPHER M JONES

Diagnostic Results

VERSIONS
DMT: 2.00
PIC: 2.05
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.0°C
Breath Tube = 46.9°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.63 V
Cooler Voltage = 1.67 V
Bias Voltage = 80 V
Chopper Freq = 554 Hz

PUMP INFO

Flow Rate = 4.463 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.1673	0.1701
MIN (V)	0.1654	0.1687

FILTER INFO

Filter 1	0.169	Zero = true
Filter 2	0.462	Zero = true
Filter 3	1.528	Zero = true

CALIBRATION CHECK

Xq = 0.094 0.83%

Accuracy and Precision Check

Concentration	= 0.098 g/210L
Lot #	= 16-21-100
Range	= 0.093 - 0.103
Average	= 0.098 g/210L
Std Dev	= 0.0000

RF Detection Test

Failed

*Triggered By operator By
Mistake, Hit cancel button*

C MJ

Routine Performance Check Failed

Performed by

C MJ

Date

02/24/2017

Reviewed by

Date

DATAMASTER DMT MAINTENANCE LOG

Colchester Police
Department/Agency

DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
2/24/17	<p>DMT External Standard Solution Lot # 16-21-100 EtOHaq Conc: 0.098 Range: 0.093 - 0.103 Preparation Date: 9/13/2016 Expires: 9/13/2017</p> <p>[For RP Preparation Date: 9/13/2016 Expires: 9/13/2017 OPENED: 2-24-17 CMS ice Label Here]</p> <p style="font-size: 1.2em; font-family: cursive;">RPC / Solution Change</p>	<p style="font-size: 1.5em; font-family: cursive;">CMS MIS</p>
	<p>[For RPC or Simulator Solution Change Place Label Here]</p>	
	<p>[For RPC or Simulator Solution Change Place Label Here]</p>	
	<p>[For RPC or Simulator Solution Change Place Label Here]</p>	
	<p>[For RPC or Simulator Solution Change Place Label Here]</p>	