

INSTALLATION REPORT

DataMaster DMT: 100157
Location: COLCHESTER PD
Calibration Date: 04/11/2017
Certification Date: 04/11/2017
Installation Date: 04/11/2017
Installed by: DAVID PATLAK



Default Options Loaded

Diagnostic Results

VERSIONS
DMT: 2.03
PIC: 2.05
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.9°C
Breath Tube = 45.4°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.66 V
Cooler Voltage = 1.67 V
Bias Voltage = 80 V
Chopper Freq = 531 Hz

PUMP INFO

Flow Rate = 3.850 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	-0.0303	-0.0266
MIN (V)	-0.0323	-0.0289

FILTER INFO

Filter 1	-0.028	Zero = true
Filter 2	0.272	Zero = true
Filter 3	1.369	Zero = true

CALIBRATION CHECK

Xq = 0.093 0.37%

INSTALLATION PASSED

Accuracy and Precision Check


Concentration	= 0.101 g/210L
Lot #	= 17-16-100
Range	= 0.096 - 0.106
Average	= 0.099 g/210L
Std Dev	= 0.0004

RF Detection Test

Passed

Sample Acceptance Test

Passed

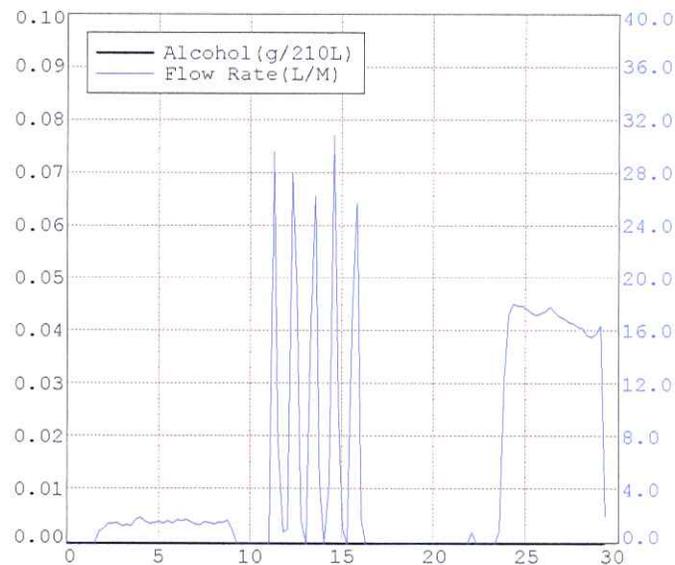

Performed by

Date

04/11/2017

Reviewed by

Date

4/17/17

DMT Serial Number #100157

Page 1 of 1

04/11/2017 5:00 PM