

Datamaster Monthly Update Checklist

Department/Agency: Colchester PD

DM serial #: 100157

Date: 7118117 for 6/1/17 - 6/30/17

	Provided	None this month
Operators Logbook	<input checked="" type="checkbox"/>	<input type="checkbox"/>
Maintenance Logbook	<input checked="" type="checkbox"/>	<input type="checkbox"/>
Breath Summary Report	<input checked="" type="checkbox"/>	<input type="checkbox"/>
Status Summary Report	<input checked="" type="checkbox"/>	<input type="checkbox"/>
Calibration	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Certification	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Installation	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Annual Preventative Maintenance	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Routine Performance Check	<input checked="" type="checkbox"/>	<input type="checkbox"/>
Simulator Solution Change	<input type="checkbox"/>	<input checked="" type="checkbox"/>
Other Reports	<input type="checkbox"/>	<input checked="" type="checkbox"/>

List other report type and date:

DATAMASTER DMT OPERATOR USE LOG

C.P.D.
Department/Agency

100157
DataMaster DMT Serial Number

Date	DMT Operator's Name	Subject's Name	Simulator Vapor 1	Simulator Vapor 2
3/8/17	Locke, Paul	Heidi Cass	.097	
3/9/17	Coulombe, Jareo	Brandon E Scarfone	.098	.096
4/2/17	GUTIERREZ, STEPHEN	KEVIN DIDENBARK	.098	
4/4/17	Jones, Chris	Evan Harwood	.098	
4/7/17	Roy, James	Jane Doe	.096	
4/7/17	Lehmann, Juelc John Doe	John Doe	.098	
4/11/17	DAVID ATLAS	TEST / INSTALL	0.099	
4/13/17	V. BITCA	Christopher Mason	0.099	
4-14-17	C. Jones	Chad Hotchkiss	.900	
4/17/17	J. Bressler	Arthur Burnier	.099	
04-21-17	M West	Nicholas Decannoy	.099	
4/22/17	V. BITCA	Anthony Brigante	.099	.098
5/3/17	FISL	Alisa Craft	.101	
05-25-17	West	Kelley Devins	.1099	.097
6-7-17	Jones	RPC	.100	
6-9-17	FISL	Ashley Traph	.1099	
6-10-17	Polandini	Harvey, Lillian	.101	
6-15-17	V. BITCA	Moran, Kelly	.100	
6/16/17	R. CURRIER	TEREK POSTSANG	.08	
7-1-17	C Jones	Amanda Reilly	.098	

DATAMASTER DMT MAINTENANCE LOG

Calchester Police

Department/Agency

DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
2/24/17	<p>DMT External Standard Solution Lot # 16-21-100 EtOHaq Conc: 0.098 Range: 0.093 - 0.103 Preparation Date: 9/13/2016 Expires: 9/13/2017</p> <p>[For RP ice Label Here]</p> <p>OPENED: 2-24-17 CMS</p> <p style="font-size: 1.5em; font-family: cursive;">RPC / Solution Change</p>	<p style="font-size: 1.5em; font-family: cursive;">CMS</p> <p style="font-size: 1.5em; font-family: cursive;">MIS</p>
4/11/17	<p>DMT Simulator Solution Lot # 17-16-100 EtOHaq Certified Conc: 0.101 Range: 0.096 - 0.106 Preparation Date: 04/03/2017 Expires: 04/03/2018</p> <p>[For RP ice Label Here]</p> <p>OPENED: 4/11/17 DJB</p> <p style="font-size: 1.5em; font-family: cursive;">INSTALL AFTER SIMULATOR UPGRADE</p>	<p style="font-size: 1.5em; font-family: cursive;">D. PATLAK</p> <p style="font-size: 1.5em; font-family: cursive;">VFL</p>
6-7-17	<p>DMT Simulator Solution Lot # 17-16-100 EtOHaq Certified Conc: 0.101 Range: 0.096 - 0.106 Preparation Date: 04/03/2017 Expires: 04/03/2018</p> <p>[For R lace Label Here]</p> <p>OPENED: 6-7-17 CMS</p> <p style="font-size: 1.5em; font-family: cursive;">RPC Solution Change</p>	<p style="font-size: 1.5em; font-family: cursive;">Clony</p> <p style="font-size: 1.5em; font-family: cursive;">6-7-17</p>
	<p>[For RPC or Simulator Solution Change Place Label Here]</p>	

Status Record History

Status Date	Status Time	Test Type	Status Message

ROUTINE PERFORMANCE CHECK REPORT



DataMaster DMT: 100157
Location: COLCHESTER PD
Calibration Date: 04/11/2017
Certification Date: 04/11/2017
Installation Date: 04/11/2017
RPC Date: 06/07/2017
Supervisor Name: CHRISTOPHER M JONES

Diagnostic Results

VERSIONS
DMT: 2.03
PIC: 2.05
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.8°C
Breath Tube = 46.9°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.66 V
Cooler Voltage = 1.67 V
Bias Voltage = 80 V
Chopper Freq = 542 Hz

PUMP INFO

Flow Rate = 3.978 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	-0.0346	-0.0319
MIN(V)	-0.0368	-0.0335

FILTER INFO

Filter 1	-0.034	Zero = true
Filter 2	0.271	Zero = true
Filter 3	1.388	Zero = true

CALIBRATION CHECK

Xq = 0.093 0.28%

Routine Performance Check Passed

Accuracy and Precision Check


Concentration = 0.101 g/210L
Lot # = 17-16-100
Range = 0.096 - 0.106
Average = 0.100 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

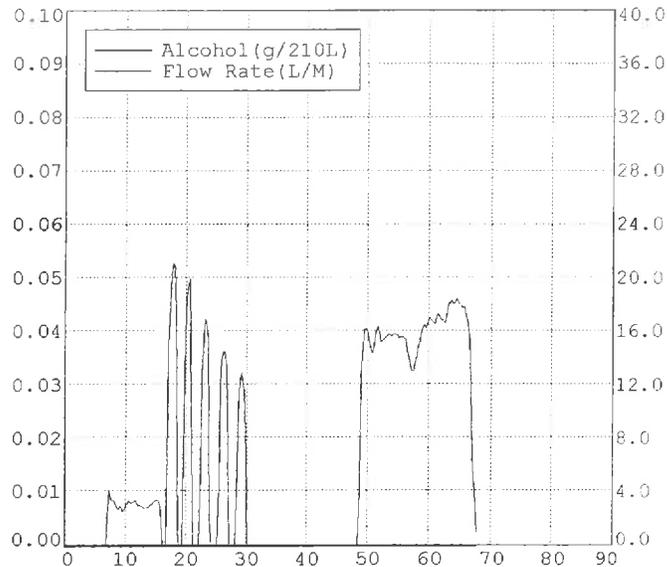

Performed by

Christopher M Jones

Date

06/07/2017

Reviewed by

Date