

INSTALLATION REPORT

DataMaster DMT: 100158
Location: NORTHFIELD PD
Calibration Date: 03/15/2017
Certification Date: 03/15/2017
Installation Date: 03/16/2017
Installed by: JEFFERY DUKETTE



Default Options Loaded

Diagnostic Results

VERSIONS
DMT: 2.03
PIC: 2.05
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.1°C
Breath Tube = 43.1°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.78 V
Cooler Voltage = 1.81 V
Bias Voltage = 80 V
Chopper Freq = 538 Hz

PUMP INFO

Flow Rate = 4.854 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.2622	0.2659
MIN (V)	0.2594	0.2636

FILTER INFO

Filter	Value	Zero
Filter 1	0.266	Zero = true
Filter 2	0.549	Zero = true
Filter 3	1.492	Zero = true

CALIBRATION CHECK

Xq = 0.092 1.25%

INSTALLATION PASSED

Accuracy and Precision Check


Concentration	= 0.101 g/210L
Lot #	= 17-10-100
Range	= 0.096 - 0.106
Average	= 0.099 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

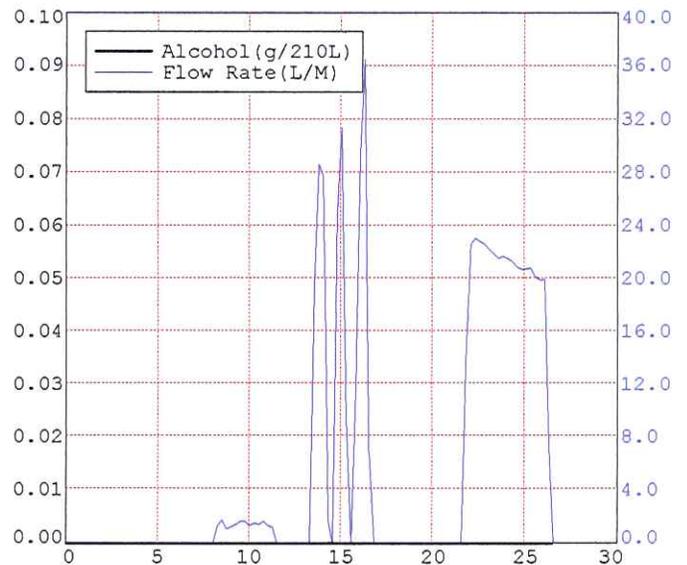

Performed by _____

350

Date _____

03/16/2017

Reviewed by _____

Date _____

3/28/17