

INSTALLATION REPORT

DataMaster DMT: 100158
Location: NORTHFIELD PD
Calibration Date: 02/23/2023
Certification Date: 02/23/2023
Installation Date: 03/22/2023
Installed by: JEFFERY DUKETTE



Default Options Loaded

Diagnostic Results

VERSIONS
DMT: 2.06
PIC: 3.07
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.9°C
Breath Tube = 43.6°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.57 V
Cooler Voltage = 1.56 V
Bias Voltage = 80 V
Chopper Freq = 551 Hz

PUMP INFO

Flow Rate = 4.820 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	-0.0803	-0.0738
MIN (V)	-0.0821	-0.0752

FILTER INFO

Filter	Value	Zero
Filter 1	-0.075	true
Filter 2	0.287	true
Filter 3	1.236	true

CALIBRATION CHECK

Xq = 0.103 1.48%

INSTALLATION PASSED

Accuracy and Precision Check


Concentration	= 0.101 g/210L
Lot #	= 23-02-100
Range	= 0.096 - 0.106
Average	= 0.099 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed
RF detected

Sample Acceptance Test

Passed

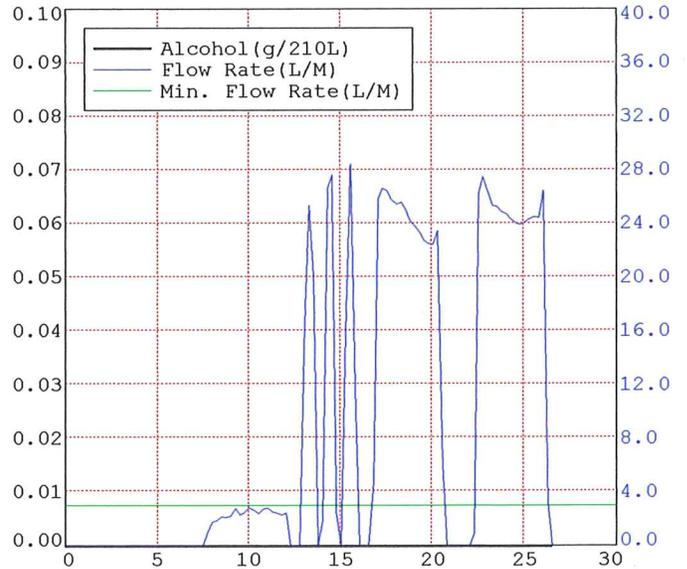

Performed by

Date

03/22/2023

Reviewed by

Date

3/27/23