

INSTALLATION REPORT

DataMaster DMT: 100160
Location: ST. ALBANS PD
Calibration Date: 10/12/2022
Certification Date: 10/12/2022
Installation Date: 10/28/2022
Installed by: JEFFERY DUKETTE



Default Options Loaded

Diagnostic Results

VERSIONS
DMT: 2.06
PIC: 2.08
Modem: 2.6
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube = 47.0°C
Digital Sim = 34.0°C

SETTINGS

Lamp Voltage = 1.67 V
Cooler Voltage = 1.66 V
Bias Voltage = 80 V
Chopper Freq = 538 Hz

PUMP INFO

Flow Rate = 5.096 L/M

DETECTOR INFO

PUMP ON OFF
MAX (V) -0.0833 -0.0762
MIN (V) -0.0852 -0.0780

FILTER INFO

Filter 1 -0.075 Zero = true
Filter 2 0.233 Zero = true
Filter 3 1.428 Zero = true

CALIBRATION CHECK

Xq = 0.085 0.60%

INSTALLATION PASSED

Accuracy and Precision Check


Concentration = 0.101 g/210L
Lot # = 22-12-100
Range = 0.096 - 0.106
Average = 0.097 g/210L
Std Dev = 0.0005

RF Detection Test

Passed
RF detected

Sample Acceptance Test

Passed

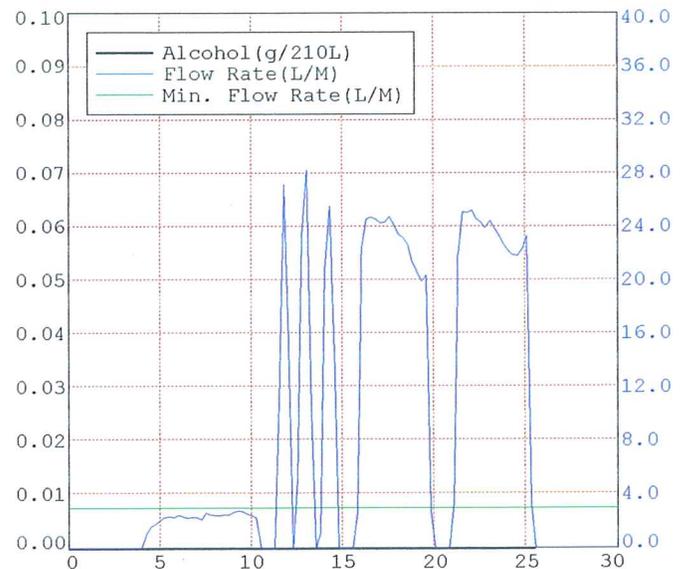

Performed by

A handwritten signature in black ink, appearing to be 'JD', is written over a horizontal line.

Date

10/28/2022

Reviewed by

A handwritten signature in blue ink, appearing to be 'JD', is written over a horizontal line.

Date

10/28/2022