VERMONT CRIMINAL JUSTICE TRAINING COUNCIL

DUI ENFORCEMENT CERTIFICATION COURSE

DRINKING EXERCISE

DS

DATE: 6-1-06 SUBJECT: — —

WEIGHT: 210 AGE: 23 TARGET BAC: .10 %

ESTIMATED OUNCES TO TARGET: 96 (8) OF ~~BEER~~ (LONG TRAIL) IN 2 HOURS

TIME	OUNCES OF	BAC (ALCOSENSOR)
1203	Long Trail	
1213	Long Trail	
1223	Long trail	
1237	Long Trail	
1253	Long Trail	
1311	Long trail	
		1332 / .085
1334	Long Trail	
		1405 .097
		1509 / .092

RELEASED TO: _____ AT _____ HOURS BAC: _____

SUPERVISOR OF DOSING _____

COMMENTS: Mouth Alc pre .109

VERMONT CRIMINAL JUSTICE TRAINING COUNCIL

DUI ENFORCEMENT CERTIFICATION COURSE

DRINKING EXERCISE

JE.

DATE: 6-1-06 SUBJECT: _____

WEIGHT: 162 AGE: 22 TARGET BAC: .10 %

ESTIMATED OUNCES TO TARGET: 72 (6) OF BEER (Heineken) IN 2 HOURS

TIME	OUNCES OF _____	BAC (ALCOSENSOR)
1202	Heineken	
1213	Heineken	
1223	Heineken	
1235	Heineken	
1253	Heineken	
1310	Heineken	
		1334/.126
		.129 1515

RELEASED TO: DEREK AT _____ HOURS BAC: _____

SUPERVISOR OF DOSING _____

COMMENTS: _____

VERMONT CRIMINAL JUSTICE TRAINING COUNCIL

DUI ENFORCEMENT CERTIFICATION COURSE

DRINKING EXERCISE

MW

DATE: 06 01 2006 SUBJECT: [illegible]

WEIGHT: 165 AGE: 27 TARGET BAC: .100 %

ESTIMATED OUNCES TO TARGET: 8 oz OF BEER IN 2 HOURS

TIME	OUNCES OF	BAC (ALCOSENSOR)
1202	1 Corona	
1209	1 Corona	
1218	1 Corona	
1230	1 Corona	
1241	1 Corona	
1302	1 Corona	1333 / .104 PBt
1334	1 Corona	1409 .124 PBt
		1514 .125 PBt

RELEASED TO: _____ AT _____ HOURS BAC: _____

SUPERVISOR OF DOSING _____

COMMENTS: 15:05 Burp

0.139 0.147

DataMaster DMT®

HPAS -- Mansfield, OH

SUBJECT TEST

National Patent
DATAMASTER dmt: 05MAY0010

Date: 6/1/2006
Time: 15:09:45

SUBJECT NAME: R W
LICENSE #:
STATE ISSUED:
DOB:

OPERATOR NAME: D M R
CERTIFICATE #:

OFFICER NAME:
ARREST LOCATION:
ARREST DATE: TIME:

Nominal = 0.102 g/210L

BLANK TEST	0.000	15:10
INTERNAL STANDARD	VERIFIED	15:10
EXTERNAL STANDARD	0.105	15:10
BLANK TEST	0.000	15:11
SUBJECT SAMPLE	0.115	15:12
BLANK TEST	0.000	15:13
SUBJECT SAMPLE	0.121	15:13
BLANK TEST	0.000	15:14

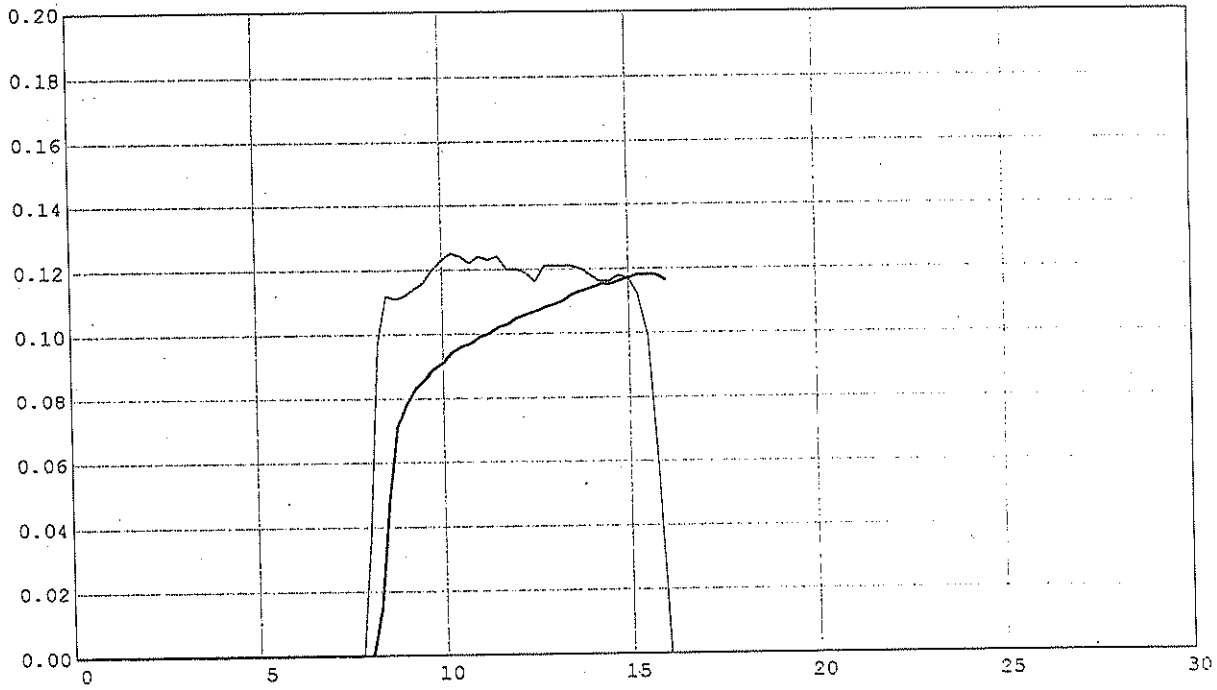

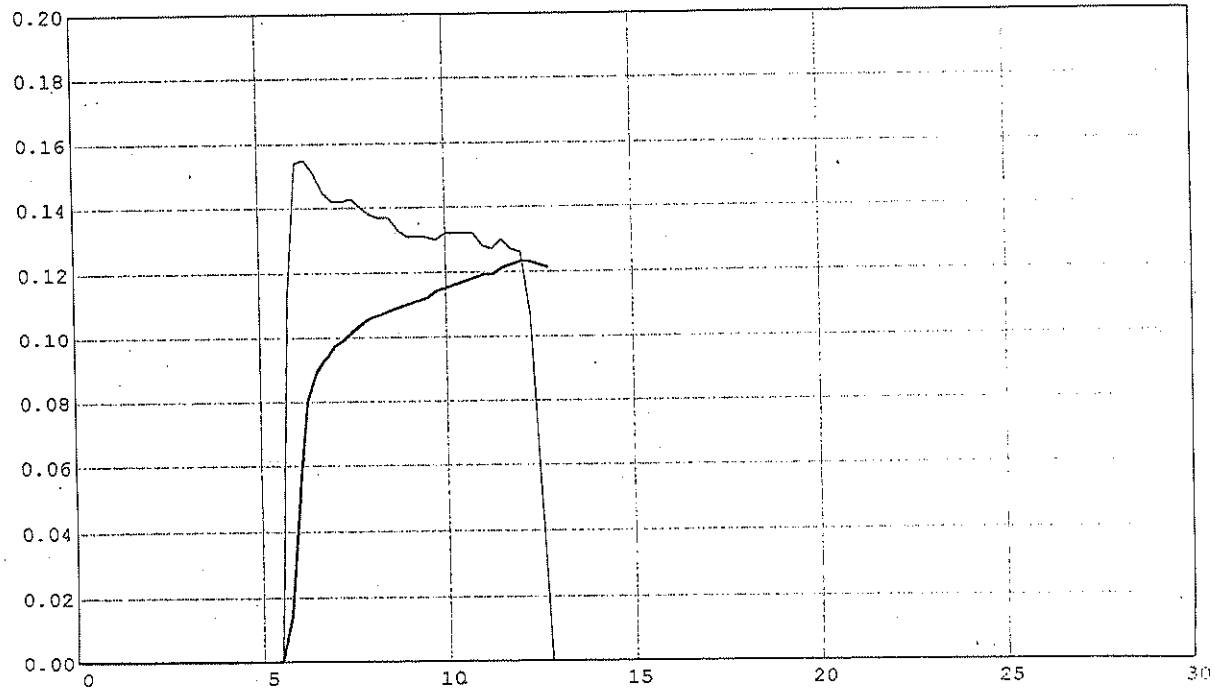

DataMaster DMT®

HPAS -- Mansfield, OH

SUBJECT TEST

National Patent
DATAMASTER dmt: 05MAY0010

Date: 6/1/2006
Time: 14:58:33

SUBJECT NAME: J M E
LICENSE #:
STATE ISSUED:
DOB:

OPERATOR NAME: D M R
CERTIFICATE #:

OFFICER NAME:
ARREST LOCATION:
ARREST DATE: TIME:

Nominal = 0.102 g/210L

BLANK TEST	0.000	14:59
INTERNAL STANDARD	VERIFIED	14:59
EXTERNAL STANDARD	0.105	14:59
BLANK TEST	0.000	15:00
SUBJECT SAMPLE	0.149	15:01
BLANK TEST	0.000	15:02

USER ABORT

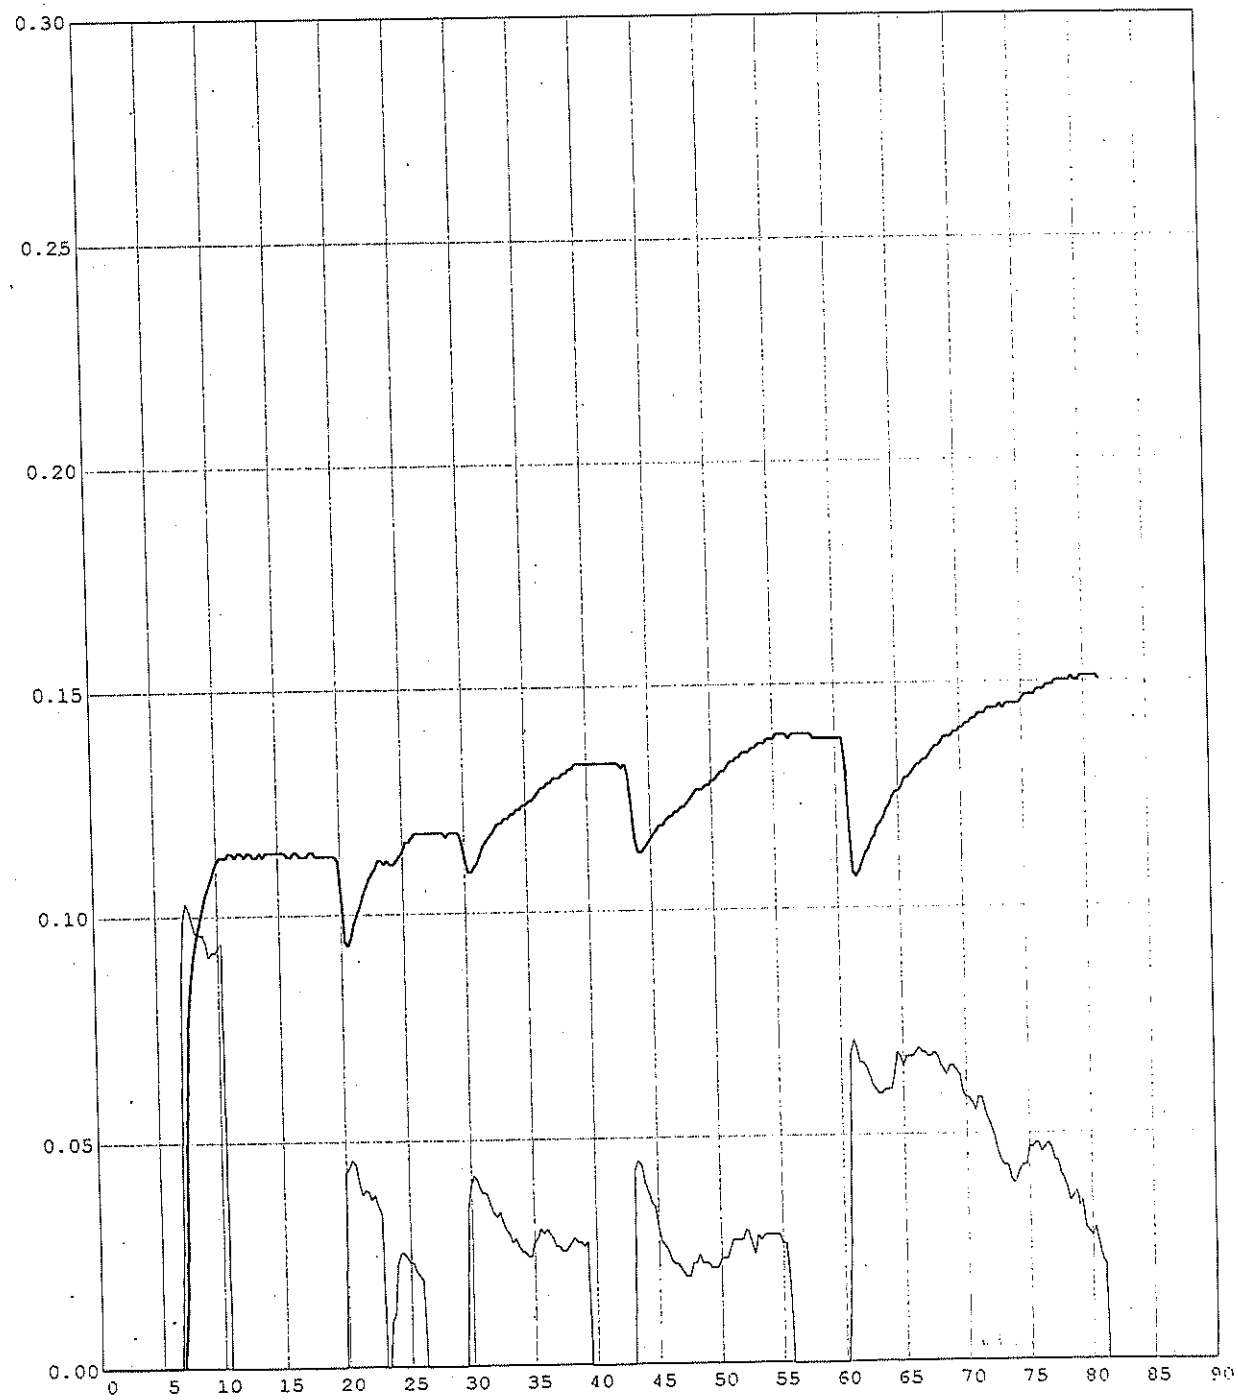

DataMaster DMT ®

NPAS -- Mansfield, OH

SUBJECT TEST

National Patent
DATAMASTER dmt: 05MAY0010

Date: 6/1/2006
Time: 14:45:36

SUBJECT NAME: L A W
LICENSE #:
STATE ISSUED:
DOB:

OPERATOR NAME: D M R
CERTIFICATE #:

OFFICER NAME:
ARREST LOCATION:
ARREST DATE: TIME:

Nominal = 0.102 g/210L

BLANK TEST	0.000	14:46
INTERNAL STANDARD	VERIFIED	14:46
EXTERNAL STANDARD	0.105	14:46
BLANK TEST	0.000	14:47
SUBJECT SAMPLE	0.102	14:47
BLANK TEST	0.000	14:48
SUBJECT SAMPLE	0.104	14:49
BLANK TEST	0.000	14:49

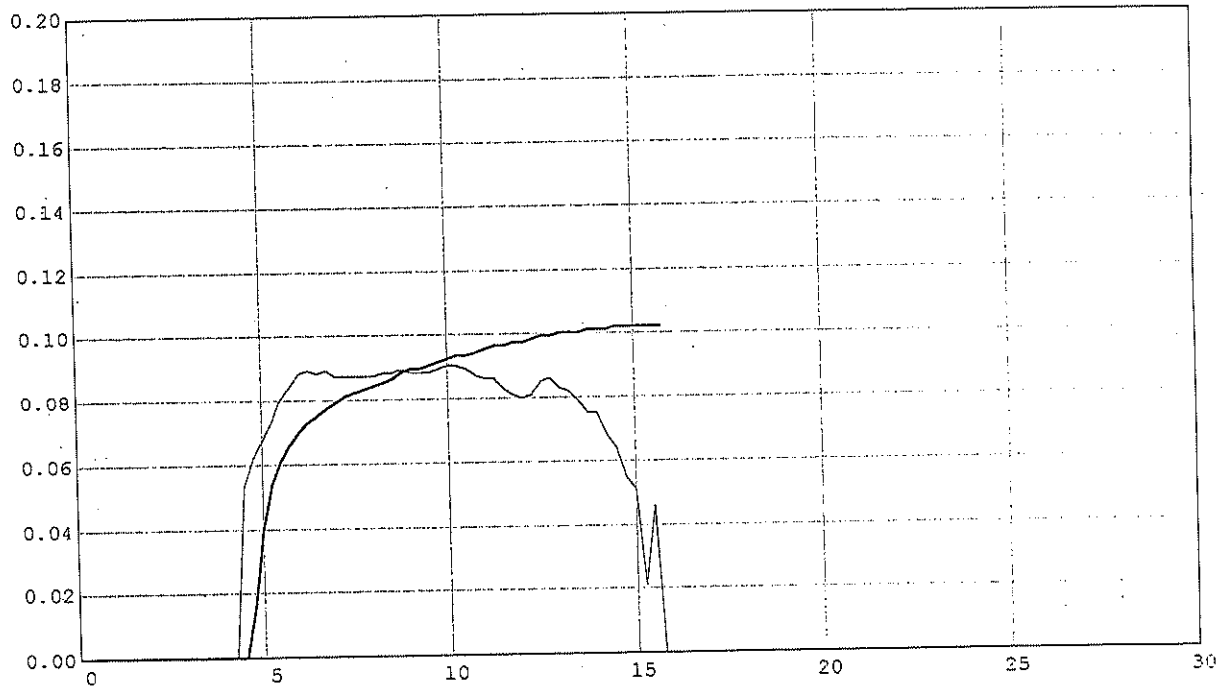

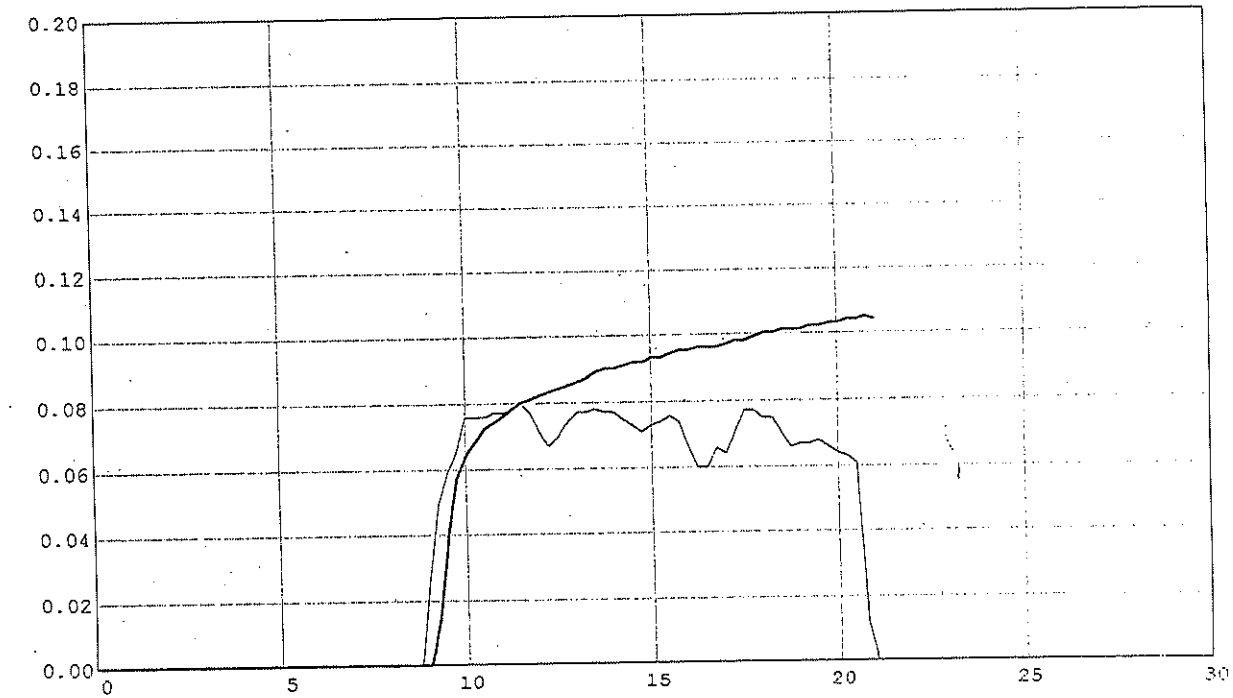

DataMaster DMT®

NPAS - Mansfield, OH

SUBJECT TEST

National Patent
DATAMASTER dmt: 05MAY0010

Date: 6/1/2006
Time: 14:26:45

SUBJECT NAME: D J S
LICENSE #:
STATE ISSUED:
DOB:

OPERATOR NAME: D M R
CERTIFICATE #:

OFFICER NAME:
ARREST LOCATION:
ARREST DATE: TIME:

Nominal = 0.102 g/210L

BLANK TEST	0.000	14:27
INTERNAL STANDARD	VERIFIED	14:27
EXTERNAL STANDARD	0.105	14:28
BLANK TEST	0.000	14:28
SUBJECT SAMPLE	0.109	14:29
BLANK TEST	0.000	14:30
SUBJECT SAMPLE	INVALID	14:30

AMBIENT FAIL

.109 pre-mouthwash

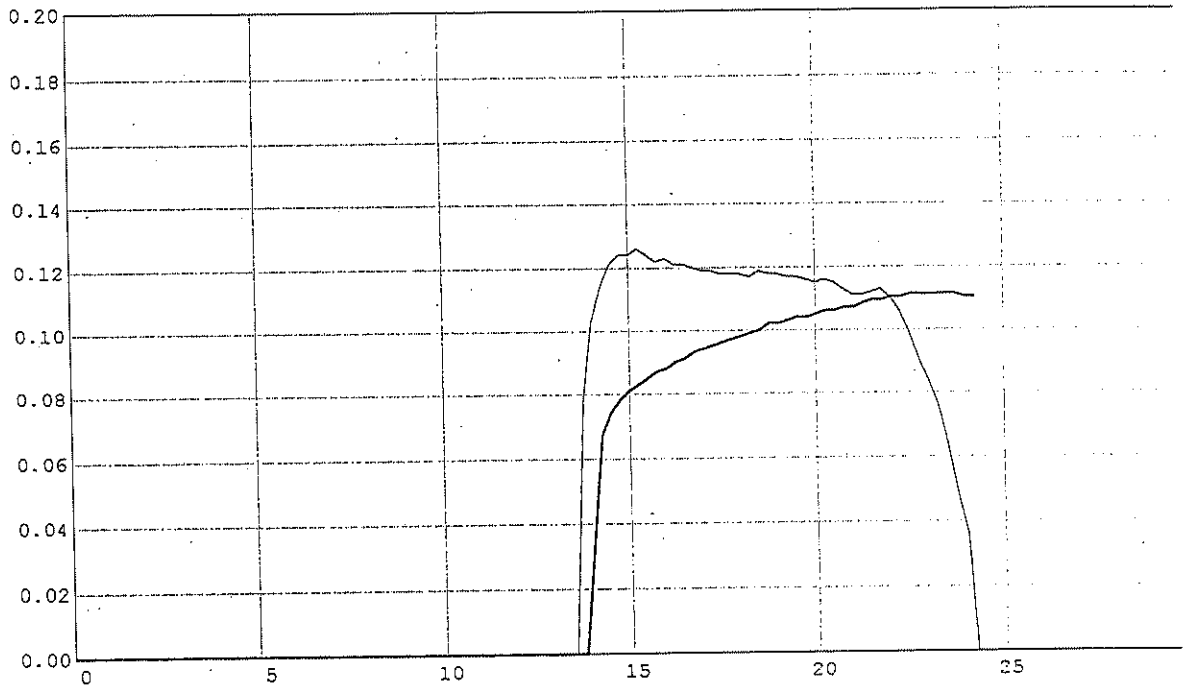

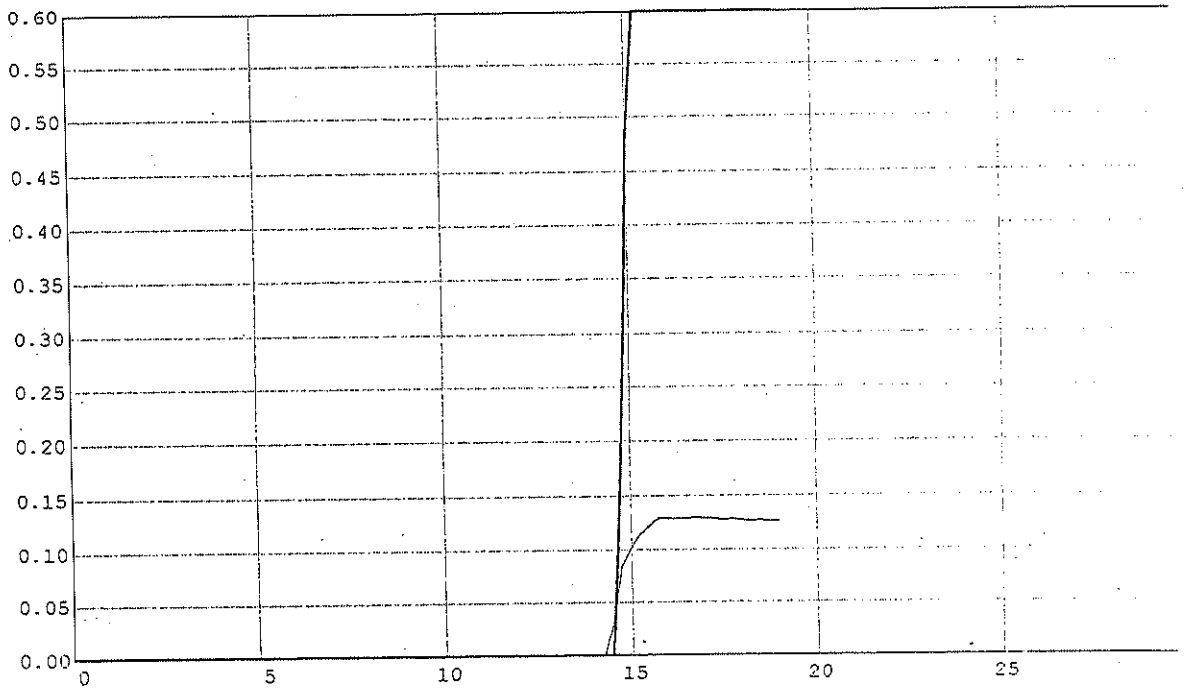

DataMaster
DMT ®
HPAS - Mansfield, OH

SUBJECT TEST

National Patent
DATAMASTER dmt: 05MAY0010

Date: 6/1/2006
Time: 13:16:27

SUBJECT NAME: R A S
LICENSE #:
STATE ISSUED:
DOB:

OPERATOR NAME: A L B
CERTIFICATE #:

OFFICER NAME:
ARREST LOCATION:
ARREST DATE: TIME:

Nominal = 0.102 g/210L

BLANK TEST	0.000	13:17
INTERNAL STANDARD	VERIFIED	13:17
EXTERNAL STANDARD	0.105	13:17
BLANK TEST	0.000	13:18
SUBJECT SAMPLE	INVALID	13:18
BLANK TEST	0.000	13:19

USER ABORT

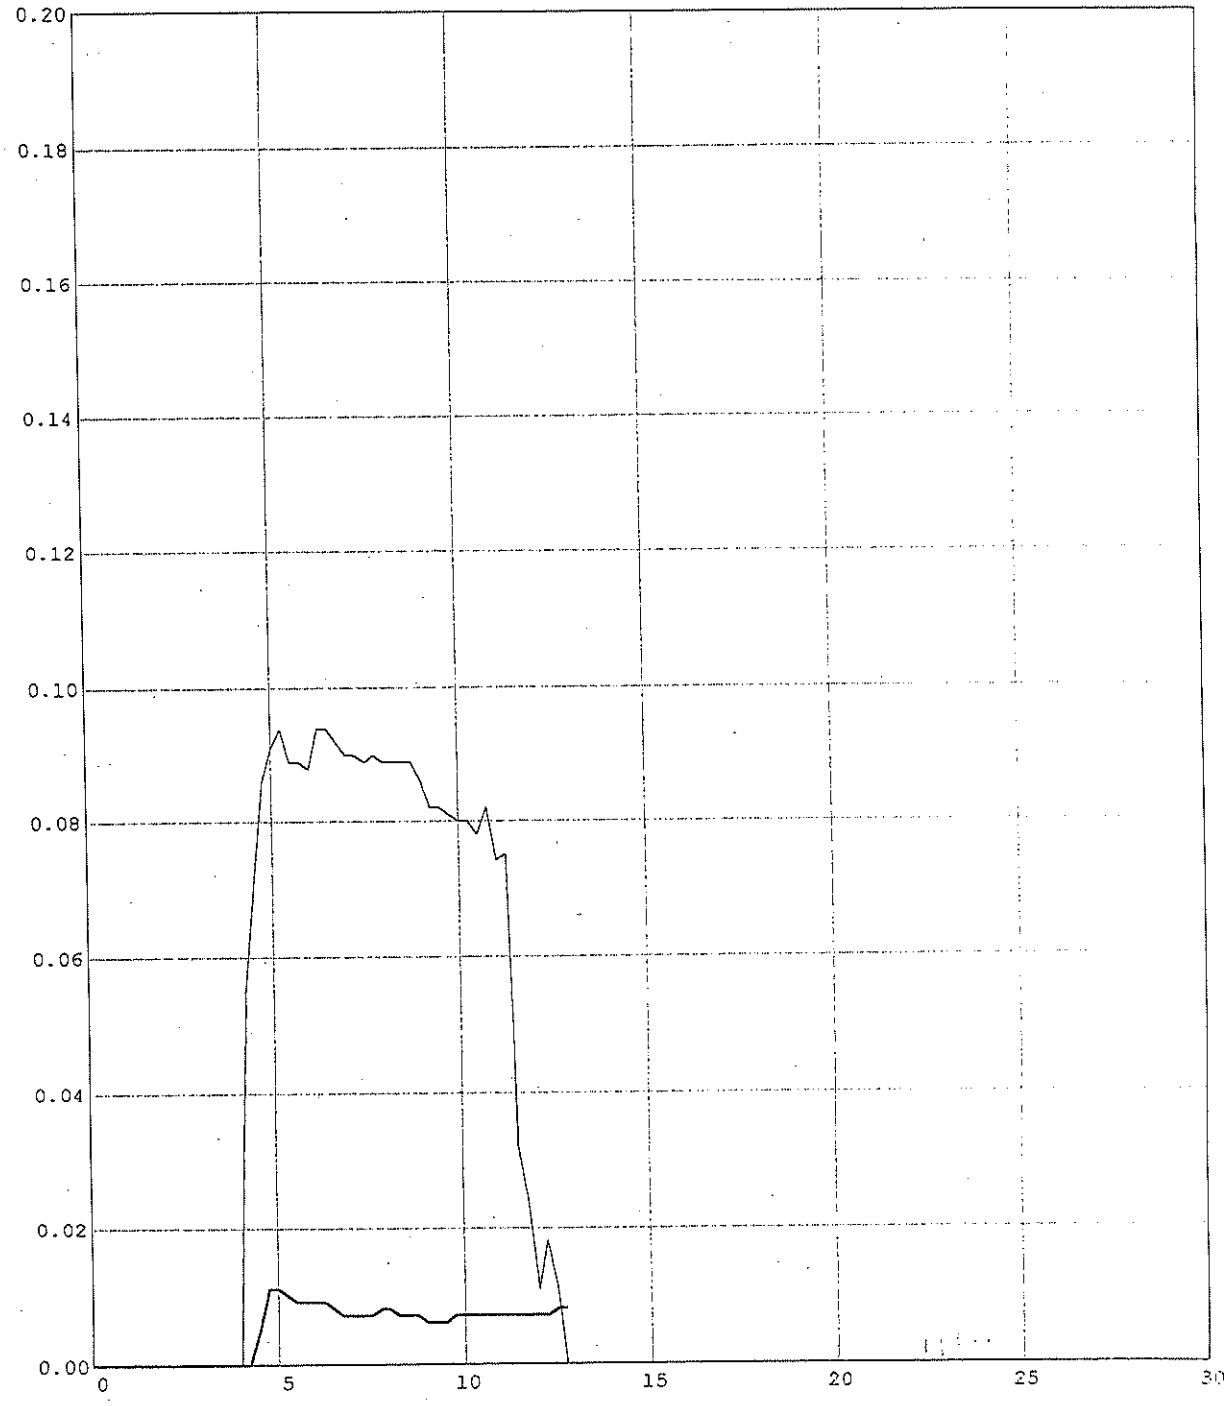

DataMaster DMT®

NPAS – Mansfield, OH

SUBJECT TEST

National Patent
DATAMASTER dmt: 05MAY0010

Date: 6/1/2006
Time: 11:38:33

SUBJECT NAME: TEST A A
LICENSE #:
STATE ISSUED:
DOB:

OPERATOR NAME:
CERTIFICATE #:

OFFICER NAME:
ARREST LOCATION:
ARREST DATE: TIME:

Nominal = 0.102 g/210L

BLANK TEST	0.000	11:39
INTERNAL STANDARD	VERIFIED	11:39
EXTERNAL STANDARD	0.104	11:39
BLANK TEST	0.000	11:40
SUBJECT SAMPLE	0.000	11:40
BLANK TEST	0.000	11:41
SUBJECT SAMPLE	0.000	11:42
BLANK TEST	0.000	11:43

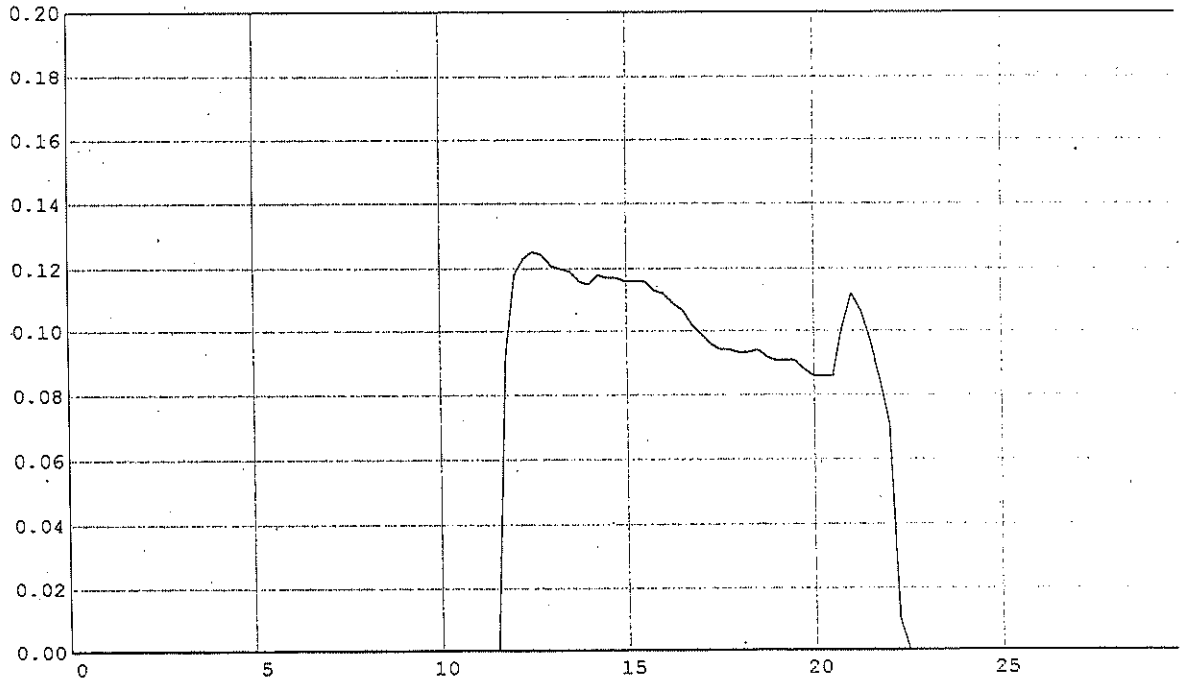

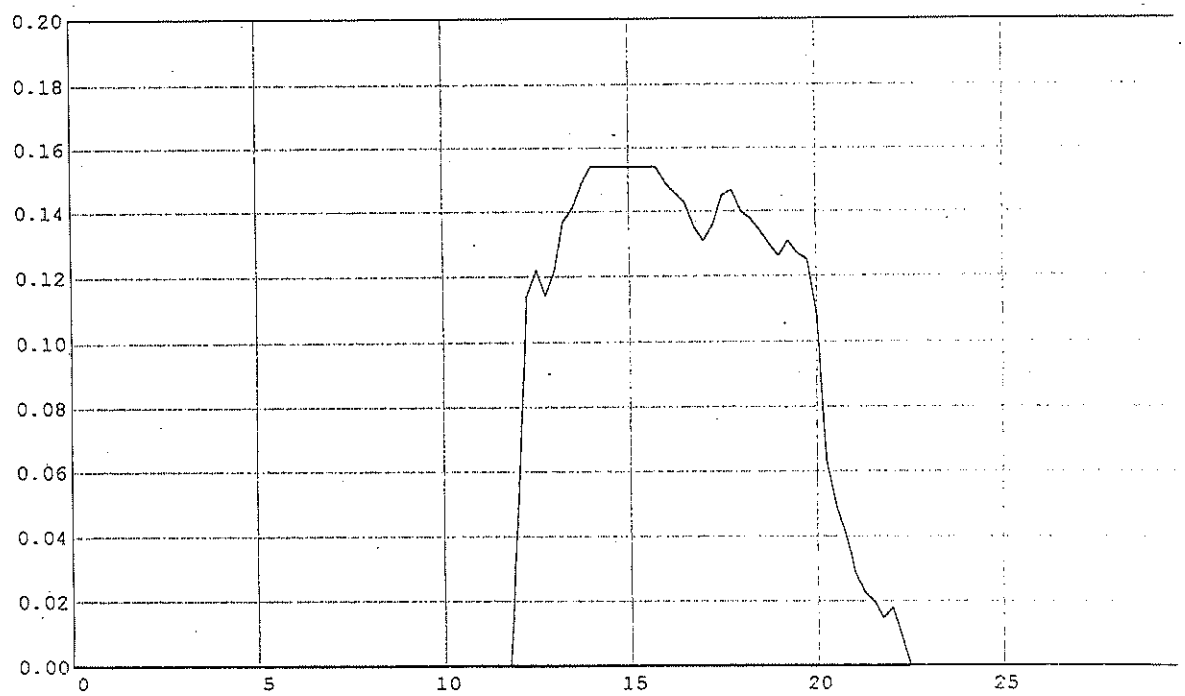

DataMaster DMT ®

NPAS – Mansfield, OH

SUPERVISOR TEST

National Patent
DATAMASTER dmt: 05MAY0010

Date: 6/1/2006
Time: 09:43:25

SUPERVISOR NAME: A L B
CERTIFICATE #:

LOT #:
BOTTLE #:
EXPIRATION:

Nominal = 0.102 g/210L

BLANK TEST	0.000	09:44
INTERNAL STANDARD	VERIFIED	09:44
EXTERNAL STANDARD	0.104	09:44
EXTERNAL STANDARD	0.105	09:45
EXTERNAL STANDARD	0.105	09:46
EXTERNAL STANDARD	0.105	09:47
EXTERNAL STANDARD	0.105	09:48
BLANK TEST	0.000	09:49

Average = 0.1048
Std Dev = 0.0004
S.E. = 2.75

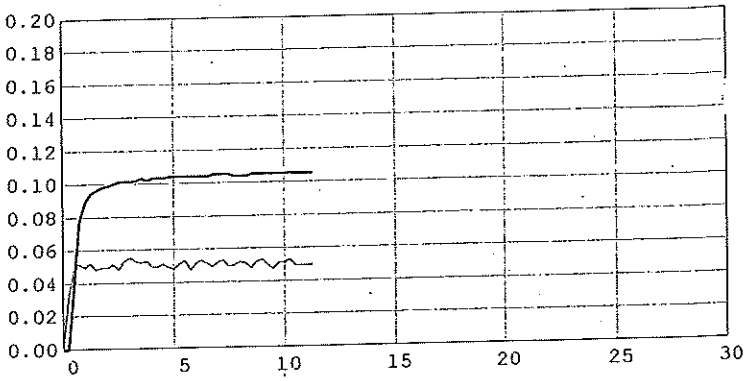

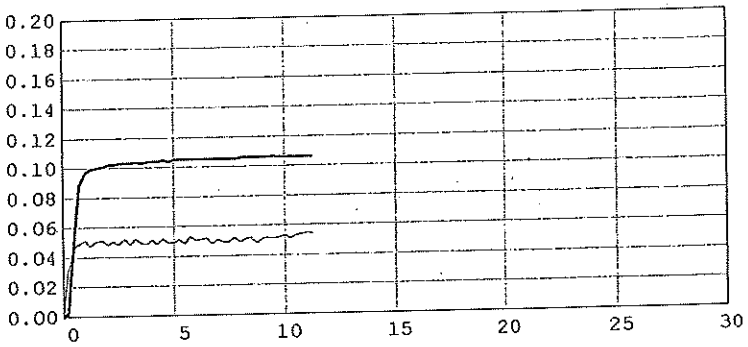

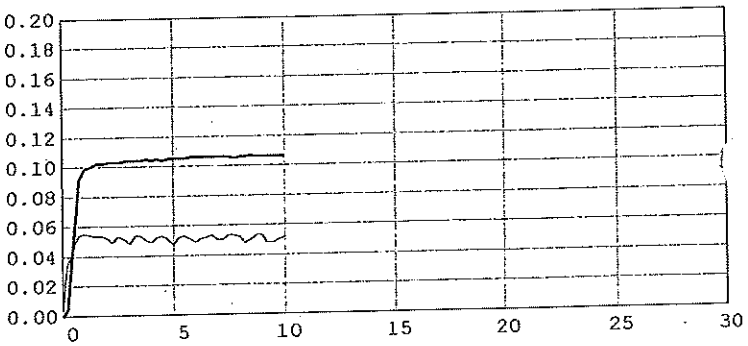

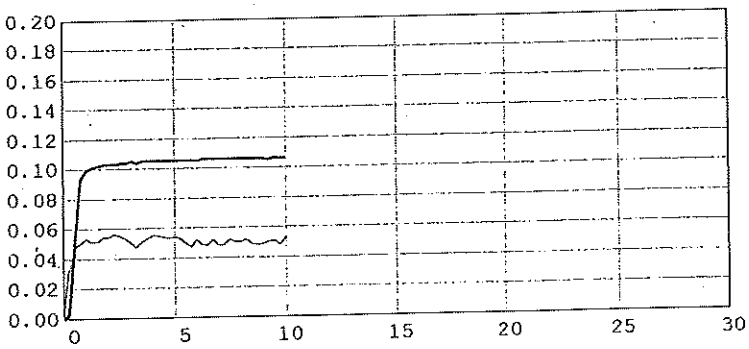

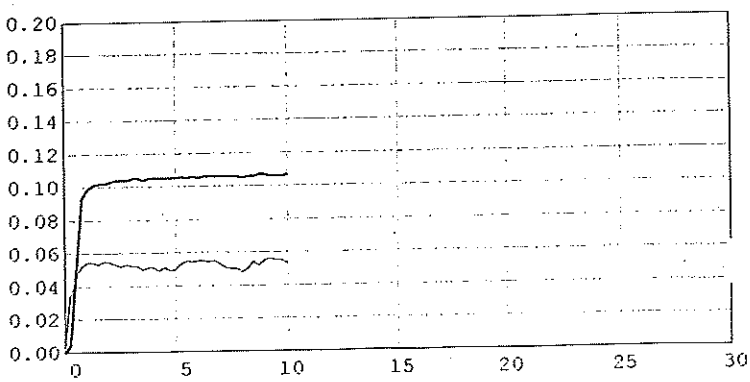

Subject Information:

080306-1:	38y	Female	161lbs	Light Beer
080306-2:	38y	Female	150lbs	Wine
080306-3:	28y	Male	199lbs	Scotch
080306-4:	37y	Male	240lbs	Rum

Test Information:

1.	080306-1	3 min after last drink	PBT: 0.071	DMT: 0.110	
2.	080306-1	Burp before blow		DMT: 0.077	
3.	080306-2	Just finished last drink	PBT: 0.071	DMT: 0.096	
4.	080306-2	Burp before blow		DMT: 0.073	
5.	080306-3	7 min after last drink	PBT: 0.087	DMT: 0.108	
6.	080306-3	Burp before blow		DMT: 0.088	
7.	080306-4	3 min after last drink	PBT: 0086	DMT: 0.124	
8.	080306-4	Burp before blow, laughing		DMT: 0.091	
9.	080306-1	Finished last drink	PBT: 0.112	DMT: 0.130	Time: 1353
10.	080306-1	Burp before blow		DMT: 0.105	Time: 1356
11.	080306-1			DMT: 0.116	Time: 1400
12.	080306-1			DMT: 0.113	Time: 1403
13.	080306-4	Finished last drink @1340		DMT: 0.093	Time: 1408
14.	080306-4	Burp before blow		DMT: 0.103	Time: 1411
15.	080306-1	Blow-suck-blow	PBT: 0.089	DMT: 0.095	
16.	080306-2	Suck-stop-blow-laugh	PBT: 0.075	DMT: 0.077	
17.	080306-3	Shallow Breath	PBT: 0.082	DMT: 0.085	
18.	080306-4	Shallow/Intermittent	PBT: 0.061	DMT: 0.058	

Spoke w/ NPAS re: performance of DMT instrument
Were informed this specific instrument is a
demo model not set up to capture accurate
samples. All tests from this instrument are
invalid 9/12/06 [illegible]

VERMONT CRIMINAL JUSTICE TRAINING COUNCIL

DUI Enforcement Certification Course

Drinking Exercise

Date: August 3, 2006 Subject: 080306-2

Weight: 150 lbs. Age: 38 Target BAC: .10 %

Estimated ounces to target: 24 of Wine in 2 hours

TIME	OUNCES OF Wine	BAC (ALCOSENSOR)
1220 Hrs.	Wine 4oz	—
1230 Hrs.	4oz	
1240 Hrs	4oz	
1250 Hrs.	4oz	
1259 Hrs.	4oz	
1310 Hrs.	—	.073%
1314 Hrs	4oz	
1322 Hrs.	4oz	
1335 Hrs	4oz	
1354 Hrs.	—	.082%
1410 Hrs.	—	.092%
1435 Hrs.	—	.088%
1505 Hrs	—	.086%
1538 hrs	—	.075%

Released to: _____ at _____ hours BAC: _____

Supervisor of Dosing: _____

Comments: _____

Rev. 2/97

VERMONT CRIMINAL JUSTICE TRAINING COUNCIL

DUI Enforcement Certification Course

Drinking Exercise

Date: August 3, 2000 Subject: [redacted] 080306-4

Weight: 240 lbs. Age: 37 Target BAC: .10 %

Estimated ounces to target: 9.5 of Rum in 2 hours

TIME	OUNCES OF Rum	BAC (ALCOSENSOR)
1220 Hrs.	Rum 1 1/4 oz	—
1230 Hrs.	1 1/4 oz	
1240 Hrs.	1 1/4 oz	
1249 Hrs.	1 1/4 oz	
1258 Hrs.	1 1/4 oz	
1307 Hrs.	1 1/4 oz	
1321 Hrs.	1 1/4 oz	.051%
1329 Hrs.	1 1/4 oz	
1335 Hrs.	1 1/4 oz	
1347 Hrs.	—	.086%
1415 Hrs	—	.087%
1440 Hrs	—	.078%
1501 Hrs	—	.070%
1536 hrs.		.061%

Released to: _____ at _____ hours BAC: _____

Supervisor of Dosing: _____

Comments: _____

Rev. 2/97

DataMaster DMT®

NPAS -- Mansfield, OH

SUBJECT TEST

National Patent
DATAMASTER dmt: 05MAY0014

Date: 8/3/2006
Time: 13:15:43

SUBJECT NAME: 080306 1
LICENSE #:
STATE ISSUED:
DOB:

OPERATOR NAME: A L B
CERTIFICATE #:

OFFICER NAME:
ARREST LOCATION:
ARREST DATE: TIME:

Nominal = 0.100 g/210L

BLANK TEST	0.000	13:16
INTERNAL STANDARD	VERIFIED	13:16
EXTERNAL STANDARD	0.104	13:17
BLANK TEST	0.000	13:17
SUBJECT SAMPLE	0.077	13:18
BLANK TEST	0.000	13:19
EXTERNAL STANDARD	0.102	13:19

USER ABORT

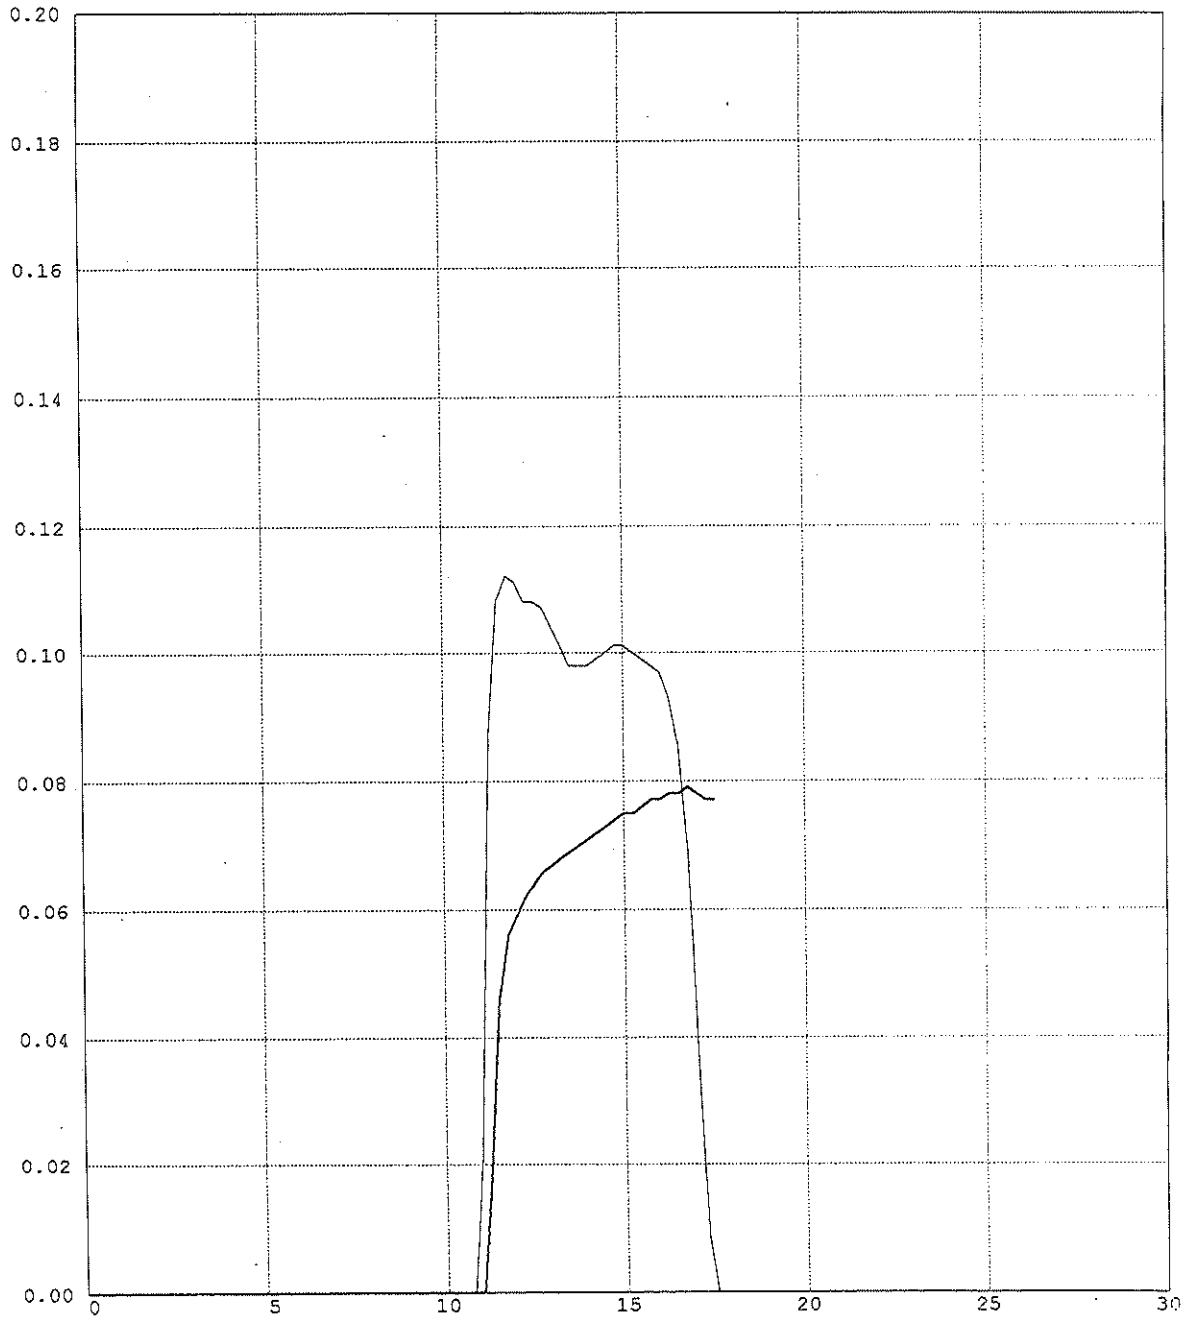

DataMaster DMT®

NPAS -- Mansfield, OH

SUBJECT TEST

National Patent
DATAMASTER dmt: 05MAY0014

Date: 8/3/2006
Time: 13:26:54

SUBJECT NAME: 080306 2
LICENSE #:
STATE ISSUED:
DOB:

OPERATOR NAME: A L B
CERTIFICATE #:

OFFICER NAME:
ARREST LOCATION:
ARREST DATE: TIME:

Nominal = 0.100 g/210L

BLANK TEST	0.000	13:27
INTERNAL STANDARD	VERIFIED	13:27
EXTERNAL STANDARD	0.104	13:28
BLANK TEST	0.000	13:29
SUBJECT SAMPLE	0.073	13:29
BLANK TEST	0.000	13:30

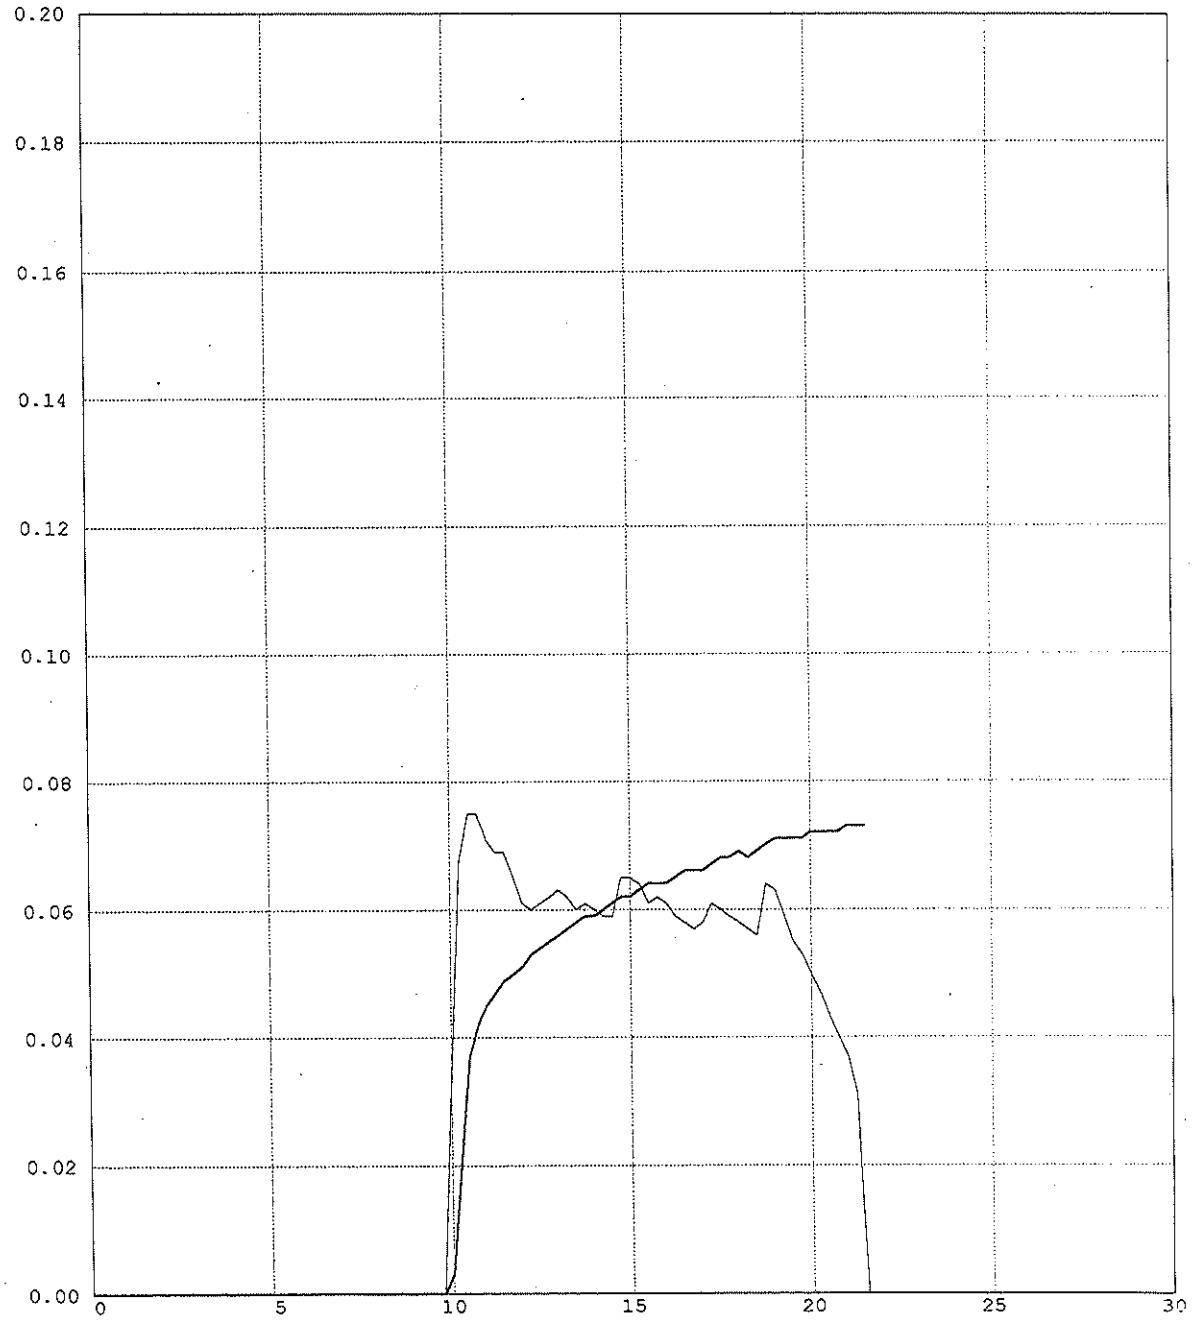

DataMaster DMT®

HPAS -- Mansfield, OH

SUBJECT TEST

National Patent
DATAMASTER dmt: 05MAY0014

Date: 8/3/2006
Time: 13:35:50

SUBJECT NAME: 080306 3
LICENSE #:
STATE ISSUED:
DOB:

OPERATOR NAME: A L B
CERTIFICATE #:

OFFICER NAME:
ARREST LOCATION:
ARREST DATE: TIME:

Nominal = 0.100 g/210L

BLANK TEST	0.000	13:36
INTERNAL STANDARD	VERIFIED	13:36
EXTERNAL STANDARD	0.102	13:37
BLANK TEST	0.000	13:38
SUBJECT SAMPLE	0.088	13:38
BLANK TEST	0.000	13:39

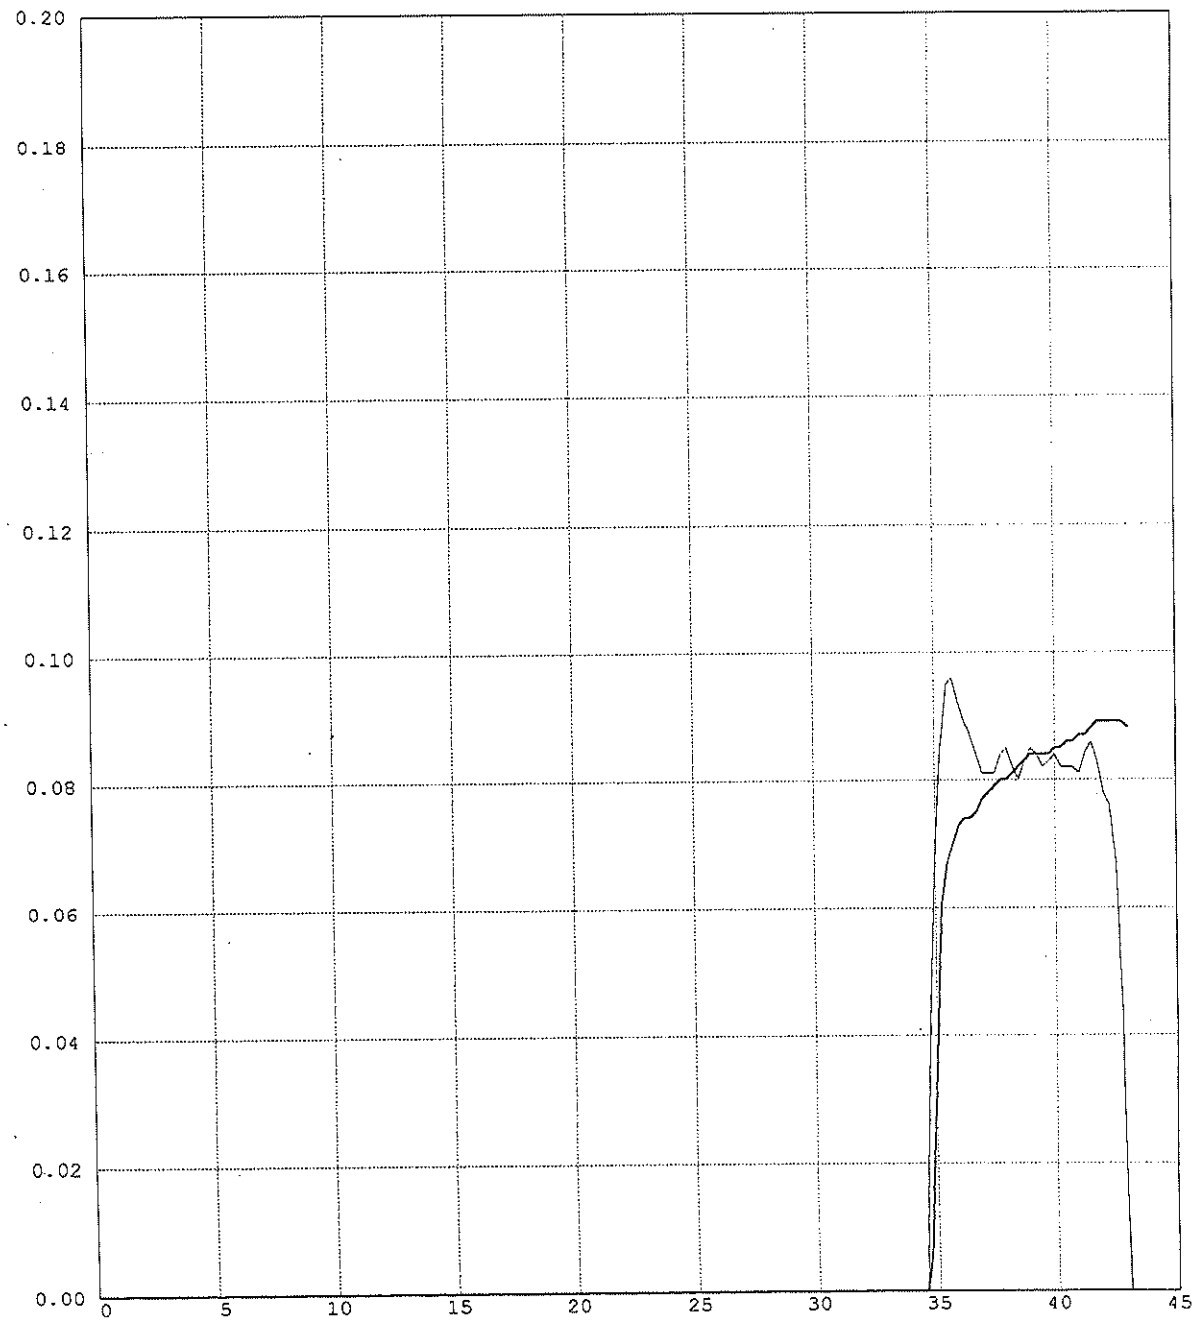

DataMaster DMT®

NPAS -- Mansfield, OH

SUBJECT TEST

National Patent
DATAMASTER dmt: 05MAY0014

Date: 8/3/2006
Time: 13:44:55

SUBJECT NAME: 080306 4
LICENSE #:
STATE ISSUED:
DOB:

OPERATOR NAME: DMR
CERTIFICATE #:

OFFICER NAME:
ARREST LOCATION:
ARREST DATE: TIME:

Nominal = 0.100 g/210L

BLANK TEST	0.000	13:45
INTERNAL STANDARD	VERIFIED	13:45
EXTERNAL STANDARD	0.103	13:46
BLANK TEST	0.000	13:47
SUBJECT SAMPLE	0.091	13:47
BLANK TEST	0.000	13:48

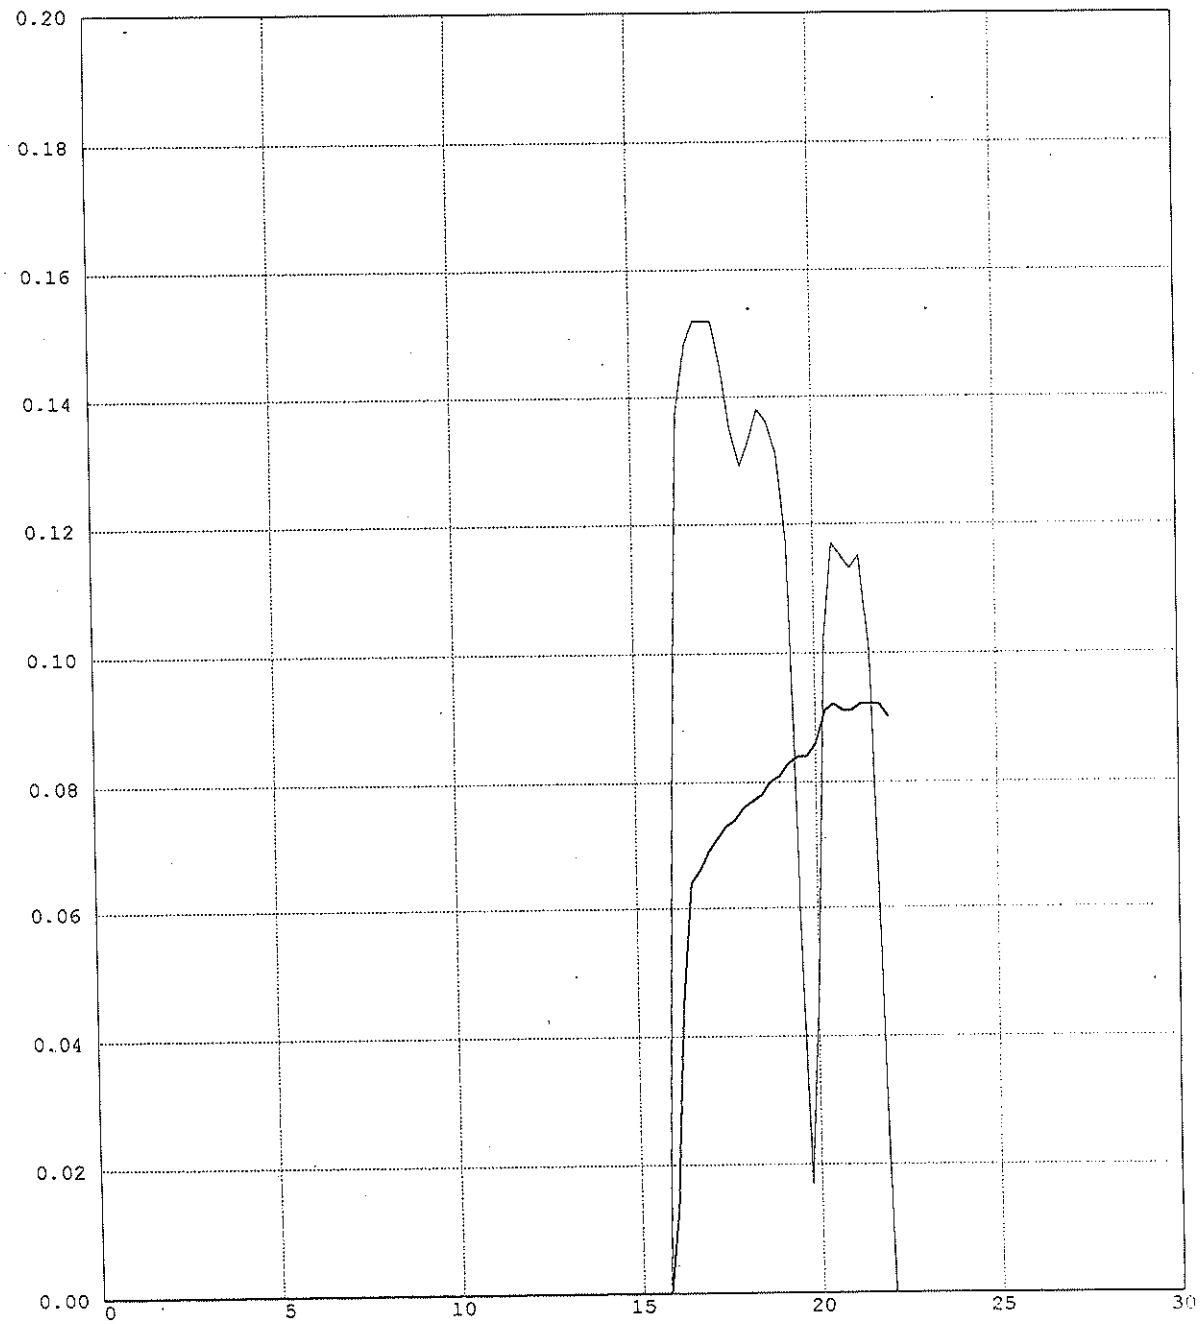

DataMaster DMT®

NPAS -- Mansfield, OH

SUBJECT TEST

National Patent
DATAMASTER dmt: 05MAY0014

Date: 8/3/2006
Time: 13:54:16

SUBJECT NAME: 080306 1
LICENSE #:
STATE ISSUED:
DOB:

OPERATOR NAME: A L B
CERTIFICATE #:

OFFICER NAME:
ARREST LOCATION:
ARREST DATE: TIME:

Nominal = 0.100 g/210L

BLANK TEST	0.000	13:55
INTERNAL STANDARD	VERIFIED	13:55
EXTERNAL STANDARD	0.101	13:55
BLANK TEST	0.000	13:56
SUBJECT SAMPLE	0.105	13:56
BLANK TEST	0.000	13:57

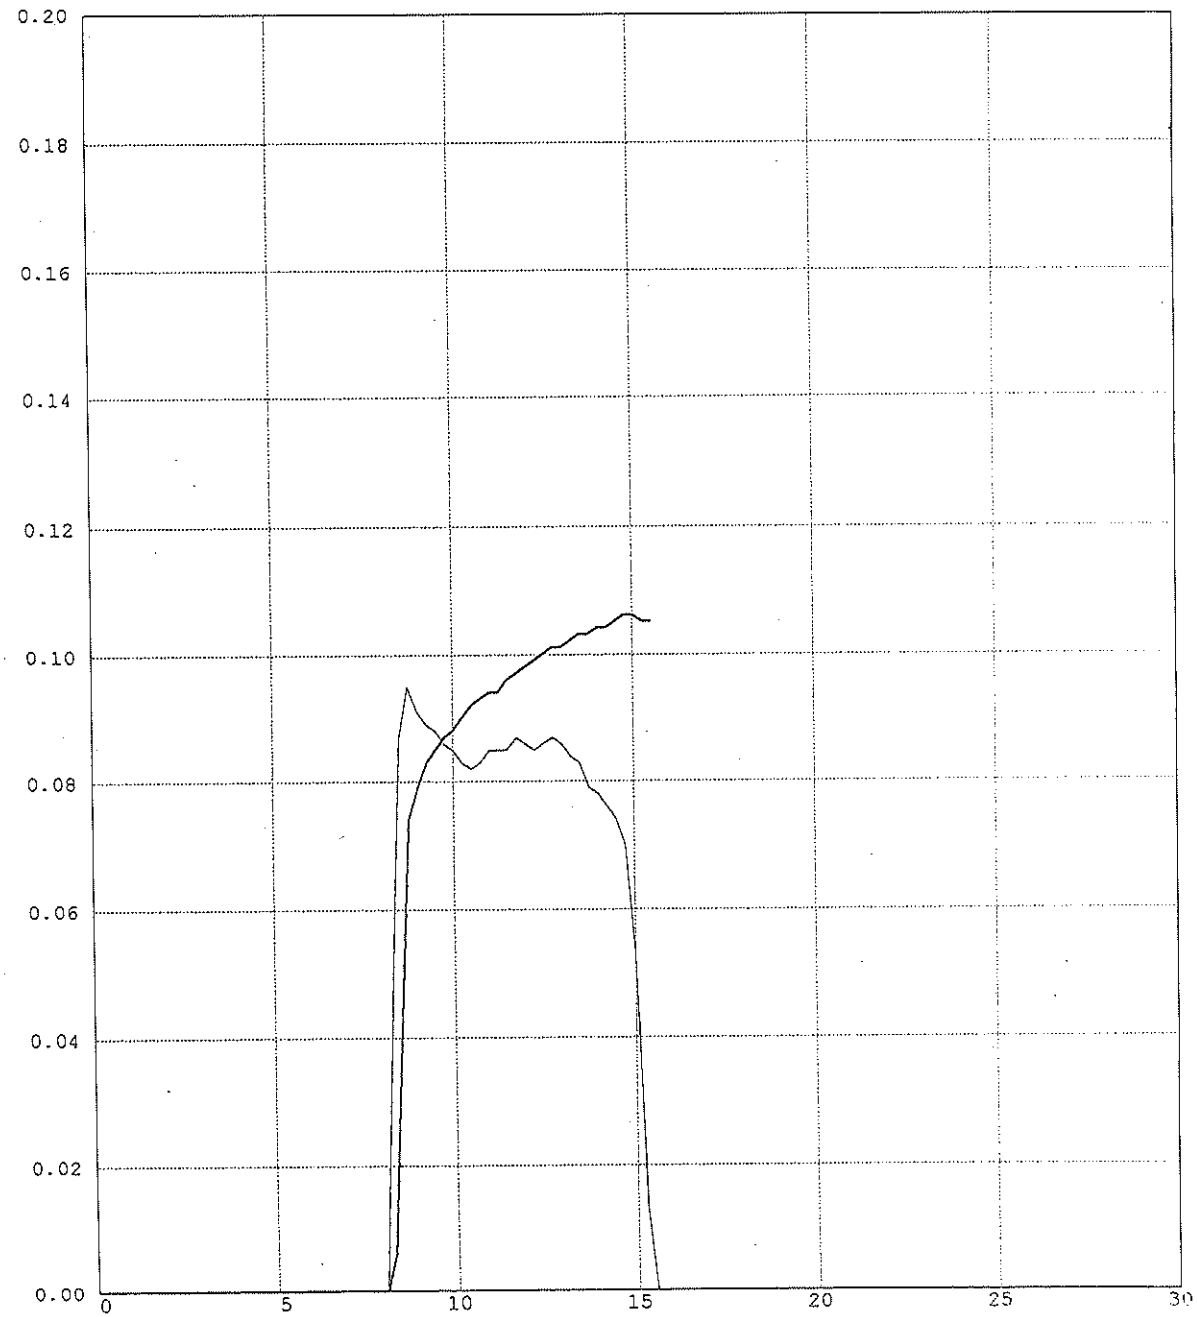

DataMaster DMT®

NPAS -- Mansfield, OH

SUBJECT TEST

National Patent
DATAMASTER dmt: 05MAY0014

Date: 8/3/2006
Time: 14:01:29

SUBJECT NAME: 080306 1
LICENSE #:
STATE ISSUED:
DOB:

OPERATOR NAME: A L B
CERTIFICATE #:

OFFICER NAME:
ARREST LOCATION:
ARREST DATE: TIME:

Nominal = 0.100 g/210L

BLANK TEST	0.000	14:02
INTERNAL STANDARD	VERIFIED	14:02
EXTERNAL STANDARD	0.104	14:02
BLANK TEST	0.000	14:03
SUBJECT SAMPLE	0.113	14:03
BLANK TEST	0.000	14:04

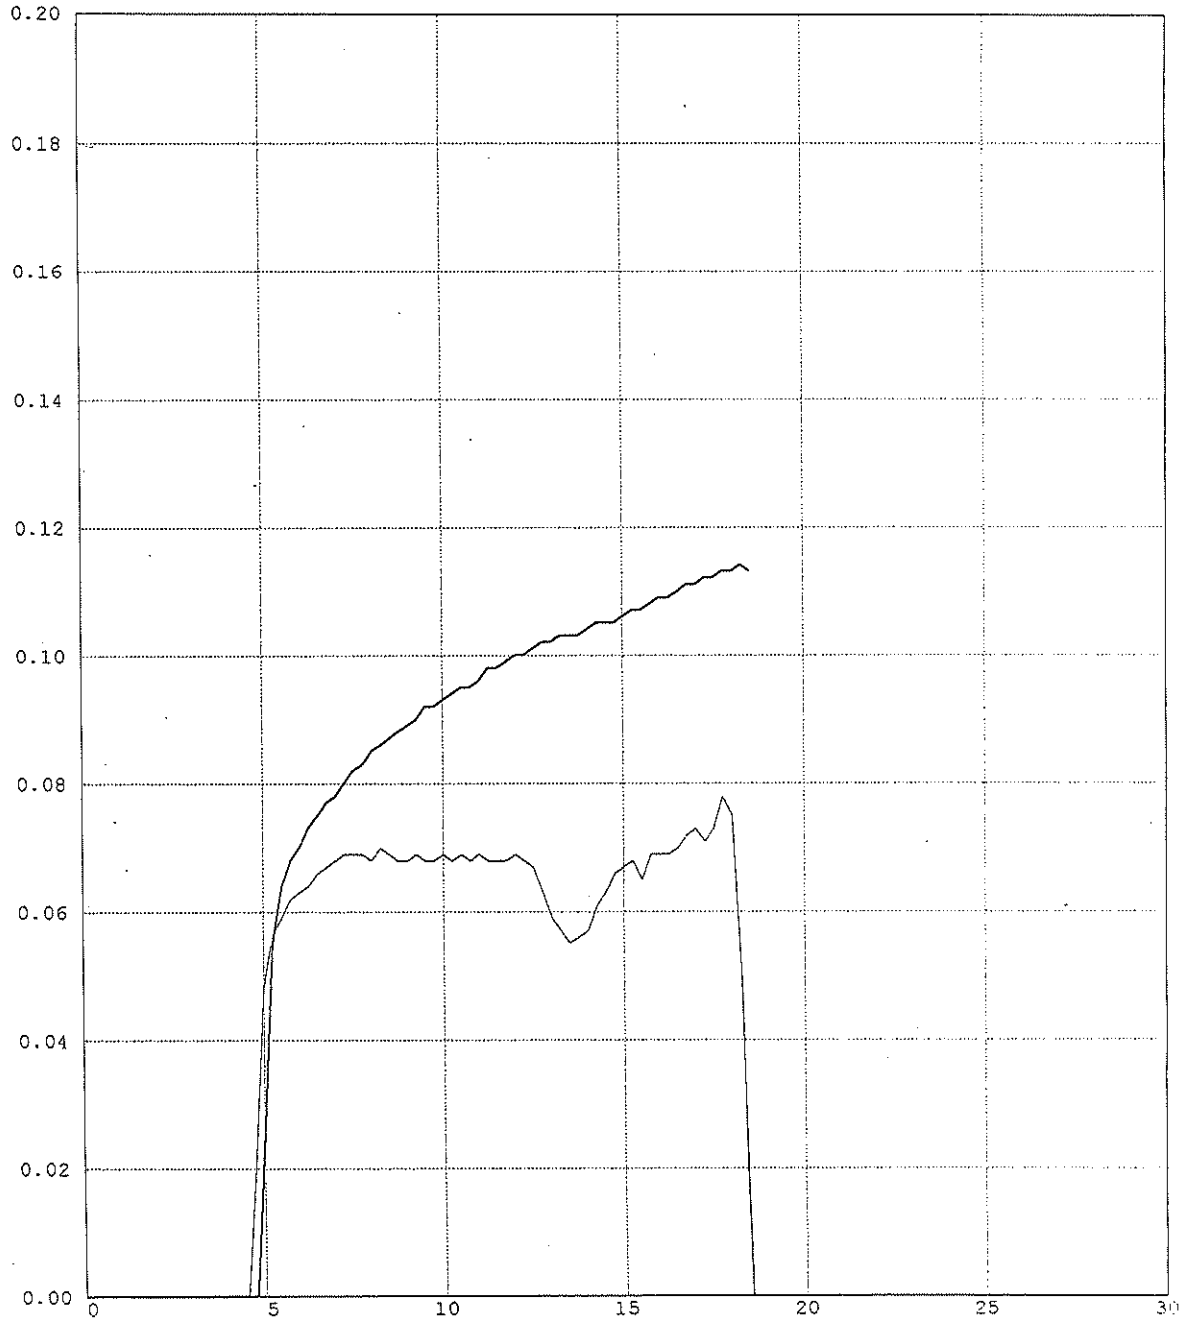

DataMaster DMT®

NPAS -- Mansfield, OH

SUBJECT TEST

National Patent
DATAMASTER dmt: 05MAY0014

Date: 8/3/2006
Time: 14:09:26

SUBJECT NAME: 080306 4
LICENSE #:
STATE ISSUED:
DOB:

OPERATOR NAME: A L B
CERTIFICATE #:

OFFICER NAME:
ARREST LOCATION:
ARREST DATE: TIME:

Nominal = 0.100 g/210L

BLANK TEST	0.000	14:10
INTERNAL STANDARD	VERIFIED	14:10
EXTERNAL STANDARD	0.103	14:10
BLANK TEST	0.000	14:11
SUBJECT SAMPLE	0.103	14:12
BLANK TEST	0.000	14:13

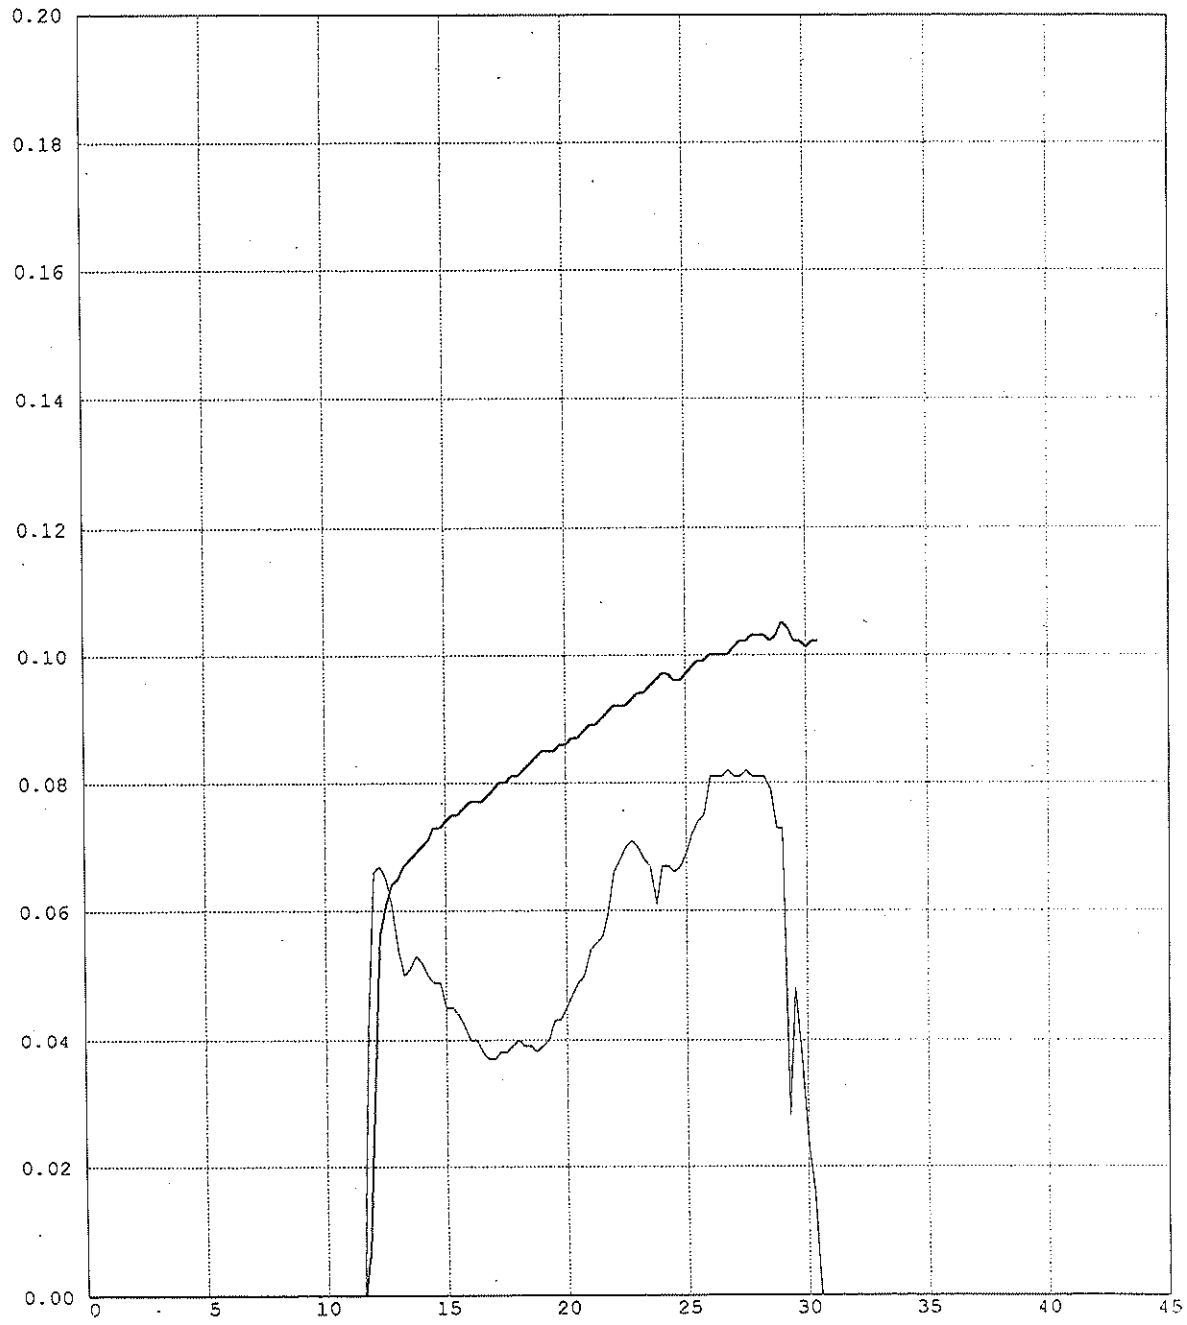

DataMaster
DMT®
HPAS -- Mansfield, OH

SUBJECT TEST

National Patent
DATAMASTER dmt: 05MAY0014

Date: 8/3/2006
Time: 15:47:46

SUBJECT NAME: 080306 2
LICENSE #:
STATE ISSUED:
DOB:

OPERATOR NAME: A L B
CERTIFICATE #:

OFFICER NAME:
ARREST LOCATION:
ARREST DATE: TIME:

Nominal = 0.100 g/210L

BLANK TEST	0.000	15:48
INTERNAL STANDARD	VERIFIED	15:48
EXTERNAL STANDARD	0.103	15:49
BLANK TEST	0.000	15:50
SUBJECT SAMPLE	0.077	15:51
BLANK TEST	0.000	15:52

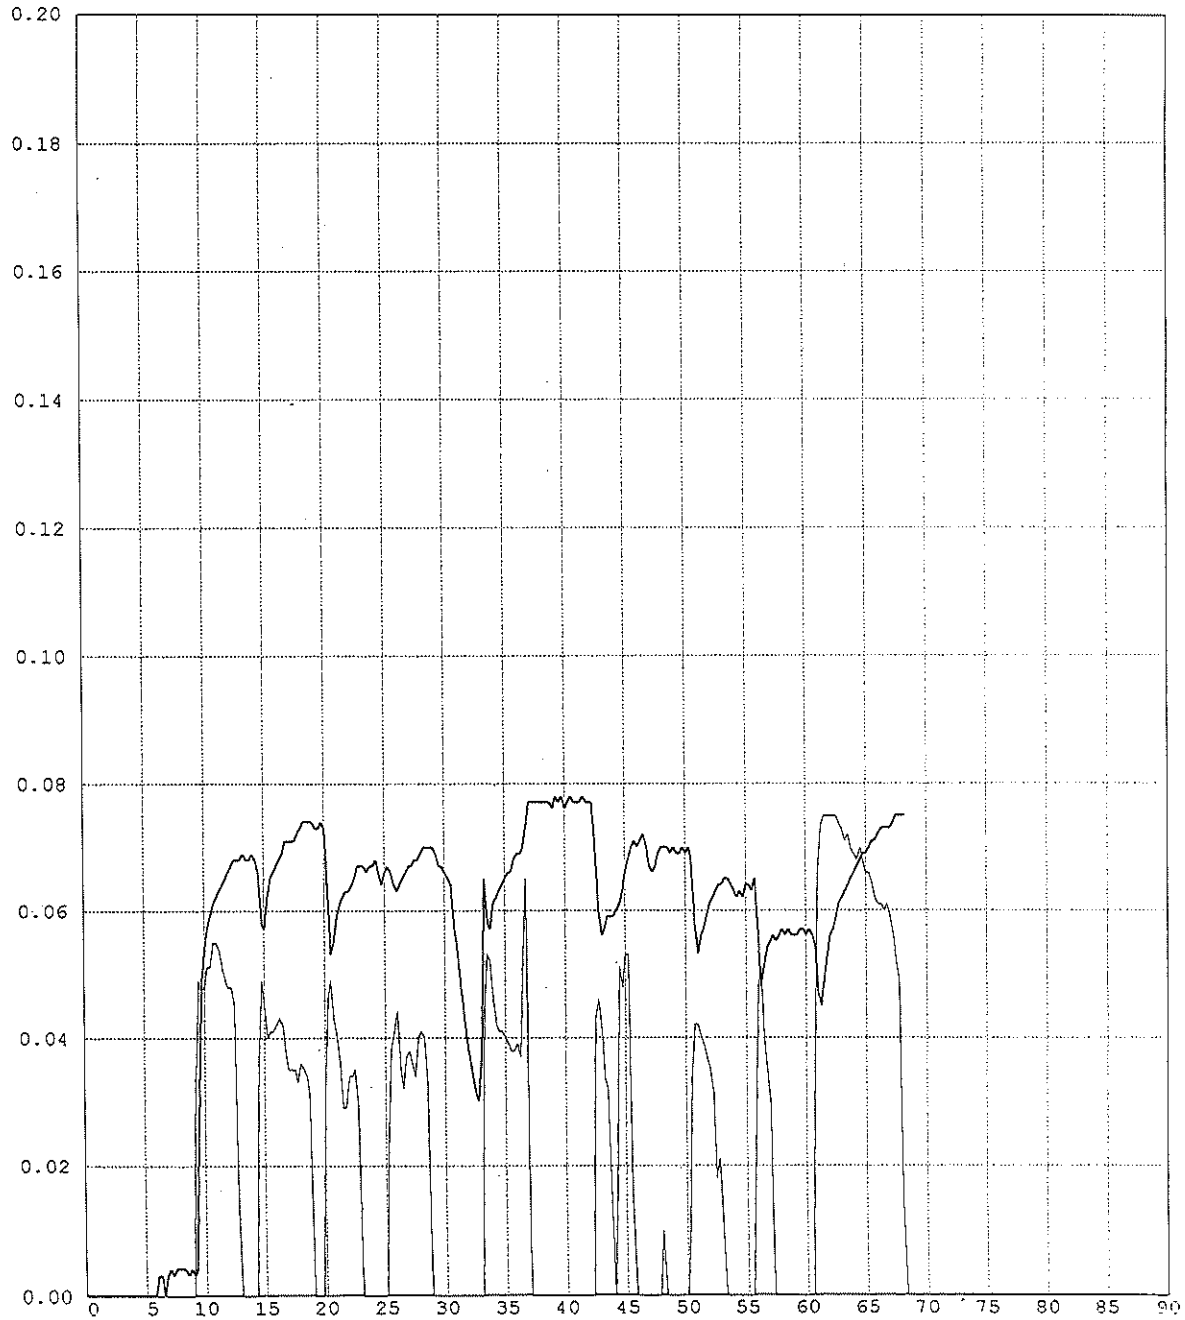

DataMaster DMT®

NPAS -- Mansfield, OH

SUBJECT TEST

National Patent
DATAMASTER dmt: 05MAY0014

Date: 8/3/2006
Time: 15:57:07

SUBJECT NAME: 080306 4
LICENSE #:
STATE ISSUED:
DOB:

OPERATOR NAME: DMR
CERTIFICATE #:

OFFICER NAME:
ARREST LOCATION:
ARREST DATE: TIME:

Nominal = 0.100 g/210L
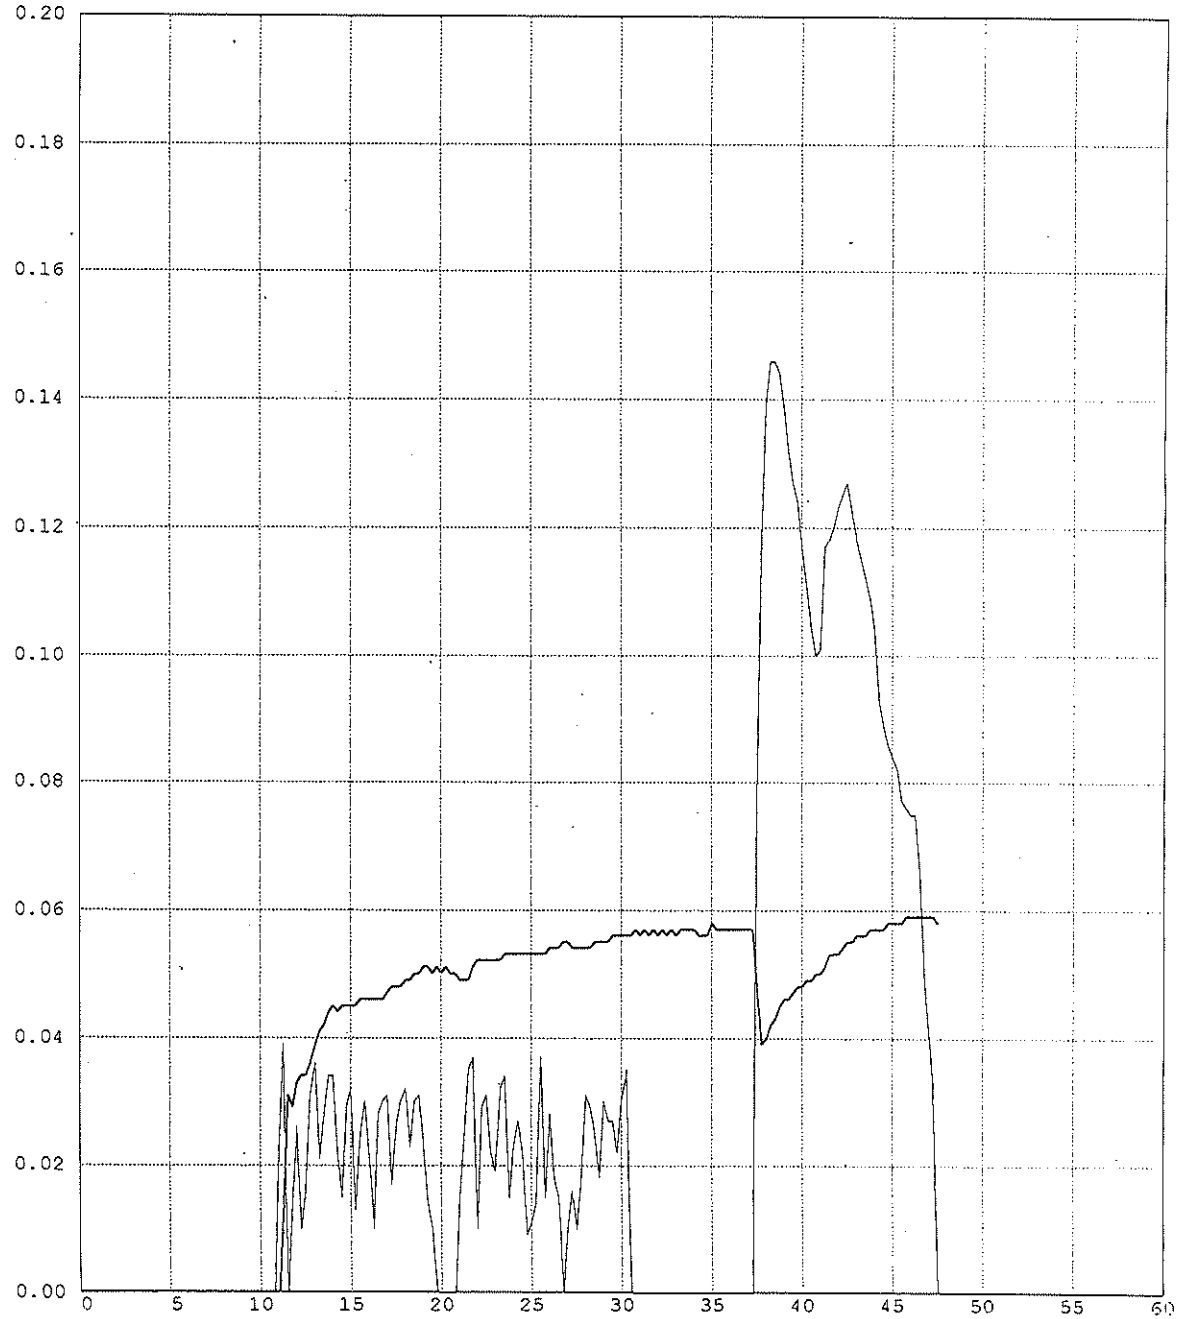
BLANK TEST	0.000	15:58
INTERNAL STANDARD	VERIFIED	15:58
EXTERNAL STANDARD	0.105	15:58
BLANK TEST	0.000	15:59
SUBJECT SAMPLE	0.058	16:00
BLANK TEST	0.000	16:01