INSTALLATION REPORT

DataMaster DMT: 122106
Location: Vergennes PD
Calibration Date: 01/03/2012
Certification Date: 01/04/2012
Installation Date: 01/12/2012
Installed by: STEVEN E HARNOIS

Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.2
Questions: 2.0

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube    = 48.1°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.72 V
Cooler Voltage = 1.79 V
Bias Voltage   = 80 V
Chopper Freq   = 528 Hz

PUMP INFO
Flow Rate = 5.101 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.0937    0.0959
MIN(V)   0.0919    0.0943

FILTER INFO
Filter 1   0.094  Zero = true
Filter 2   0.487  Zero = true
Filter 3   0.785  Zero = true

CALIBRATION CHECK
Xq  = 0.087  0.30%
```

Accuracy and Precision Check

Concentration = 0.100 g/210L
Lot # = 12-45-100
Range = 0.095 - 0.105
Average = 0.101 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

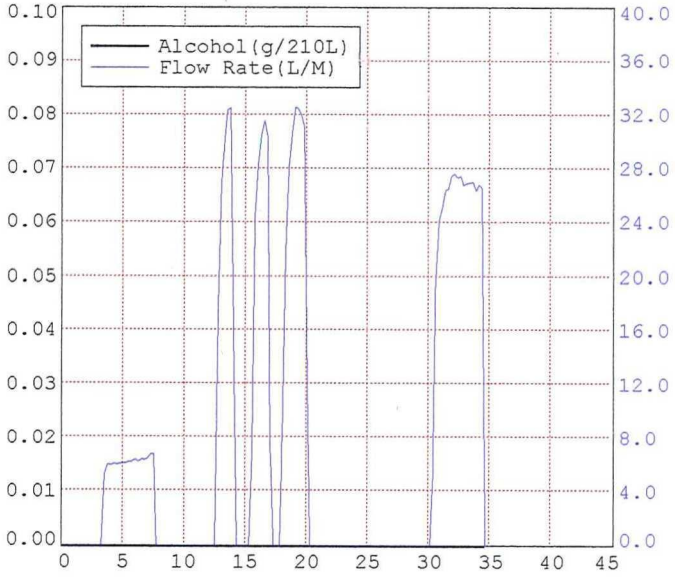

INSTALLATION PASSED

Reviewed 01/12/12

Performed by _____ Date 01/12/2012

Reviewed by _____ Date 1-12-12