INSTALLATION REPORT

DataMaster DMT: 100163
Location: Bennington County SO
Calibration Date: 09/14/2011
Certification Date: 09/15/2011
Installation Date: 10/14/2011
Installed by: STEVEN E HARNOIS

Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

VERSIONS
DMT: 1.00
PIC: 2.06
Modem: 2.1
Questions: 2.0

10/18/11 dcB

TEMPERATURES

Sample Chamber = 48.9°C
Breath Tube = 47.1°C
Digital Sim = 33.9°C

10/18/11 dcB

SETTINGS
Lamp Voltage = 1.80 V
Cooler Voltage = 1.58 V
Bias Voltage = 80 V
Chopper Freq = 548 Hz

10/18/11 dcB

PUMP INFO
Flow Rate = 5.053 L/M

10/18/11 dcB

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	-0.1797	-0.1760
MIN(V)	-0.1813	-0.1774

10/18/11 dcB

FILTER INFO
Filter 1 -0.176 Zero = true
Filter 2 0.045 Zero = true
Filter 3 0.404 Zero = true

CALIBRATION CHECK
Xq = 0.077 1.34%

Accuracy and Precision Check

Concentration = 0.102 g/210L
Lot # = 12-13-100
Range = 0.097 - 0.107
Average = 0.101 g/210L
Std Dev = 0.0000

10/18/11 dcB

RF Detection Test

Passed

10/18/11 dcB

Sample Acceptance Test

Passed

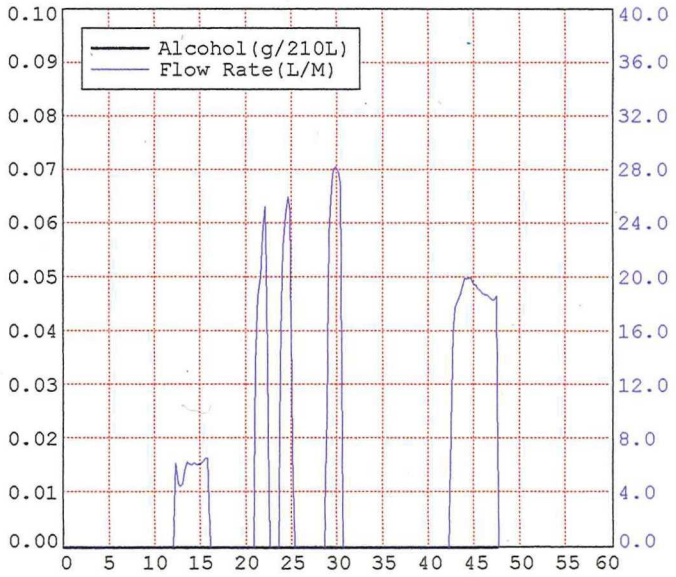

INSTALLATION PASSED

Performed by _____ Date 10/14/2011 dcB 10/18/11

Reviewed by _____ Date 10-14-11