INSTALLATION REPORT

DataMaster DMT: 100159
Location: Milton PD
Calibration Date: 12/14/2011
Certification Date: 12/14/2011
Installation Date: 12/20/2011
Installed by: STEVEN E HARNOIS

Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.2
Questions: 2.0

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube    = 48.1°C
Digital Sim    = 33.9°C

SETTINGS
Lamp Voltage   = 1.81 V
Cooler Voltage = 1.83 V
Bias Voltage   = 80 V
Chopper Freq   = 525 Hz

PUMP INFO
Flow Rate = 5.758 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   -0.1291   -0.1246
MIN(V)   -0.1307   -0.1260

FILTER INFO
Filter 1  -0.125  Zero = true
Filter 2   0.115  Zero = true
Filter 3   0.386  Zero = true

CALIBRATION CHECK
Xq  = 0.074  0.92%
```

Accuracy and Precision Check

Concentration = 0.101 g/210L
Lot # = 12-38-100
Range = 0.096 - 0.106
Average = 0.100 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

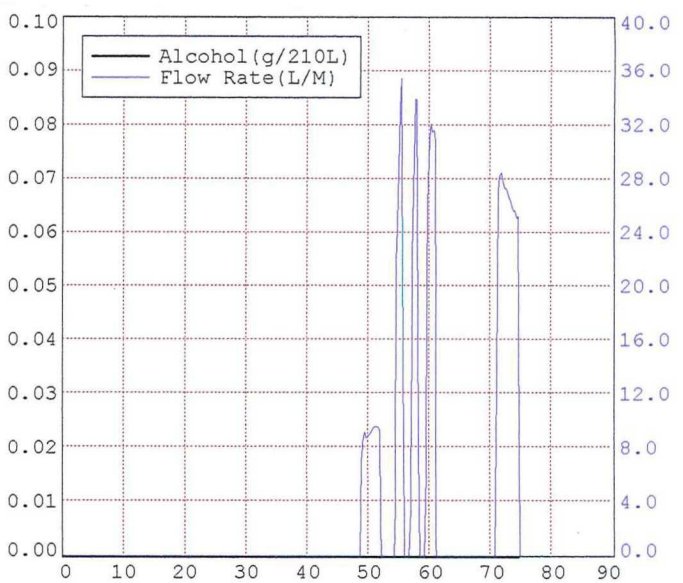

INSTALLATION PASSED

Reviewed 12-21-11

Performed by _____ Date 12/20/2011

Reviewed by _____ Date 12/20/11