INSTALLATION REPORT

DataMaster DMT: 100162
Location: South Burlington PD
Calibration Date: 11/16/2011
Certification Date: 11/17/2011
Installation Date: 12/22/2011
Installed by: KIRK L KIMBALL

Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.2
Questions: 2.0

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube    = 42.3°C
Digital Sim    = 34.1°C

SETTINGS
Lamp Voltage   = 1.82 V
Cooler Voltage = 1.80 V
Bias Voltage   = 80 V
Chopper Freq   = 527 Hz

PUMP INFO
Flow Rate = 6.122 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   -0.0994   -0.0941
MIN(V)   -0.1006   -0.0959

FILTER INFO
Filter 1  -0.095  Zero = true
Filter 2   0.284  Zero = true
Filter 3   0.936  Zero = true

CALIBRATION CHECK
Xq  = 0.075  1.25%
```

Accuracy and Precision Check

Concentration	= 0.100 g/210L
Lot #	= 12-45-100
Range	= 0.095 - 0.105
Average	= 0.098 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

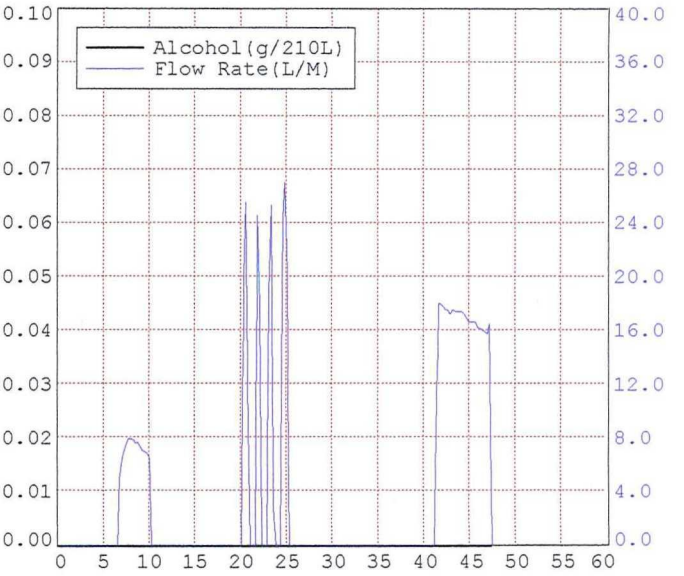

INSTALLATION PASSED

Performed by KLK Date 12/22/2011

Reviewed by Date 12/22/11

12/23/11