INSTALLATION REPORT

DataMaster DMT: 104409
Location: Winooski PD
Calibration Date: 12/19/2011
Certification Date: 12/20/2011
Installation Date: 12/23/2011
Installed by: AMANDA BOLDUC

Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.2
Questions: 2.0

TEMPERATURES

Sample Chamber = 48.9°C
Breath Tube = 47.0°C
Digital Sim = 34.0°C

SETTINGS
Lamp Voltage = 1.72 V
Cooler Voltage = 1.72 V
Bias Voltage = 80 V
Chopper Freq = 524 Hz

PUMP INFO
Flow Rate = 6.215 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX(V)	0.1098	0.1146
MIN(V)	0.1083	0.1132

FILTER INFO

Filter 1	0.114	Zero = true
Filter 2	0.353	Zero = true
Filter 3	0.470	Zero = true

CALIBRATION CHECK
Xq = 0.079 0.44%

Accuracy and Precision Check

Concentration	= 0.101 g/210L
Lot #	= 12-38-100
Range	= 0.096 - 0.106
Average	= 0.097 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

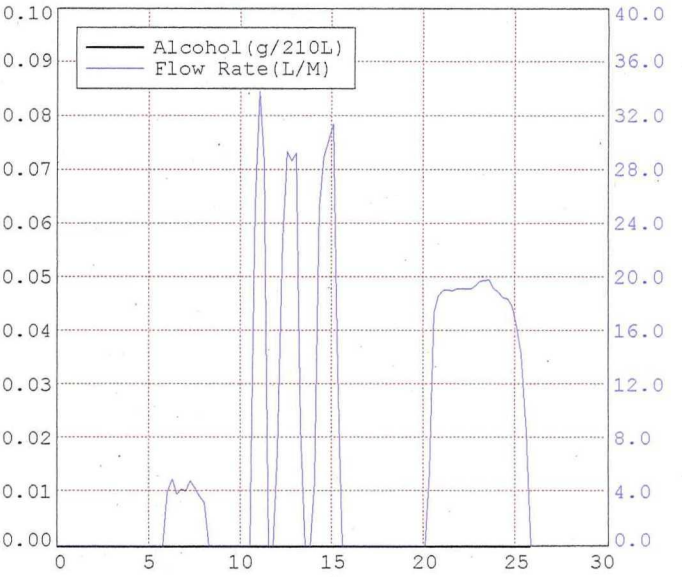

INSTALLATION PASSED

Rev. [illegible] 12-23-11

Performed by [signature] Date 12/23/2011

Reviewed by [signature] Date 12/23/11