INSTALLATION REPORT

DataMaster DMT: 104609
Location: UVM PD
Calibration Date: 12/15/2011
Certification Date: 12/16/2011
Installation Date: 12/22/2011
Installed by: KIRK L KIMBALL

Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.2
Questions: 2.0

TEMPERATURES

Sample Chamber = 49.1°C
Breath Tube    = 46.9°C
Digital Sim    = 33.9°C

SETTINGS
Lamp Voltage   = 1.75 V
Cooler Voltage = 1.70 V
Bias Voltage   = 81 V
Chopper Freq   = 534 Hz

PUMP INFO
Flow Rate = 6.150 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   -0.0404   -0.0372
MIN(V)   -0.0419   -0.0390

FILTER INFO
Filter 1  -0.039  Zero = true
Filter 2   0.284  Zero = true
Filter 3  -0.039  Zero = true

CALIBRATION CHECK
Xq  = 0.077  1.01%
```

Accuracy and Precision Check

Concentration	= 0.100 g/210L
Lot #	= 12-45-100
Range	= 0.095 - 0.105
Average	= 0.098 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

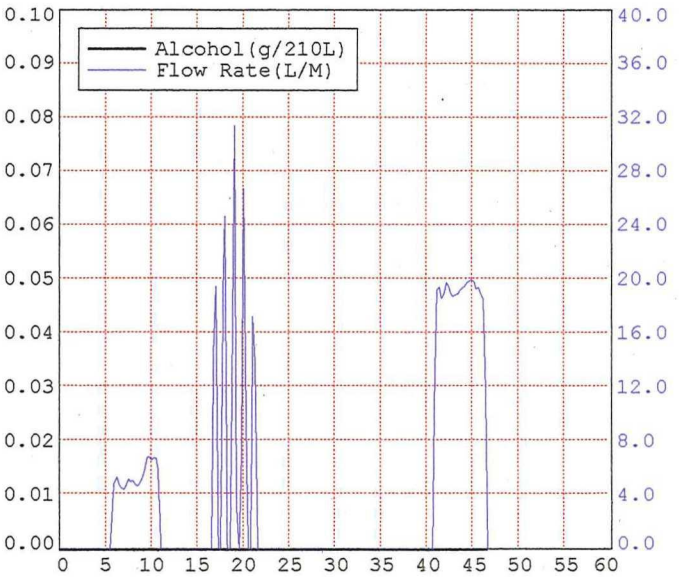

INSTALLATION PASSED

12/22/11

Performed by KLK Date 12/22/2011

Reviewed by Date 12/22/11