INSTALLATION REPORT

DataMaster DMT: 122406
Location: Essex PD
Calibration Date: 12/08/2011
Certification Date: 12/09/2011
Installation Date: 12/20/2011
Installed by: STEVEN E HARNOIS

Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.00
PIC: 2.05
Modem: 2.1
Questions: 2.0

TEMPERATURES

Sample Chamber = 49.2°C
Breath Tube    = 48.1°C
Digital Sim    = 33.8°C

SETTINGS
Lamp Voltage   = 1.80 V
Cooler Voltage = 1.77 V
Bias Voltage   = 80 V
Chopper Freq   = 533 Hz

PUMP INFO
Flow Rate = 4.636 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   -0.0309   -0.0274
MIN(V)   -0.0333   -0.0295

FILTER INFO
Filter 1  -0.028  Zero = true
Filter 2   0.880  Zero = true
Filter 3   0.908  Zero = true

CALIBRATION CHECK
Xq  = 0.091  0.48%
```

Accuracy and Precision Check

Concentration	= 0.101 g/210L
Lot #	= 12-38-100
Range	= 0.096 - 0.106
Average	= 0.098 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

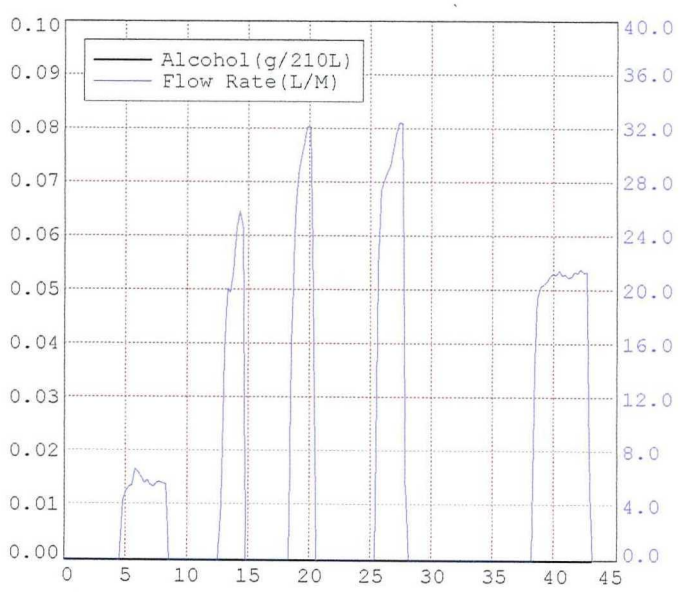

INSTALLATION PASSED

Reviewed 12-21-11

Performed by _____ Date 12/20/2011

Reviewed by _____ Date 12/20/11

DMT Serial Number #122406

12/20/2011 2:35 PM