INSTALLATION REPORT

DataMaster DMT: 100142
Location: Brandon PD
Calibration Date: 11/03/2011
Certification Date: 11/03/2011
Installation Date: 12/01/2011
Installed by: STEVEN E HARNOIS

Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.2
Questions: 2.0

TEMPERATURES

Sample Chamber = 49.1°C
Breath Tube    = 47.4°C
Digital Sim    = 34.1°C

SETTINGS
Lamp Voltage   = 1.66 V
Cooler Voltage = 1.61 V
Bias Voltage   = 80 V
Chopper Freq   = 538 Hz

PUMP INFO
Flow Rate = 5.232 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.0169    0.0213
MIN(V)   0.0154    0.0201

FILTER INFO
Filter 1   0.020  Zero = true
Filter 2   0.245  Zero = true
Filter 3   0.491  Zero = true

CALIBRATION CHECK
Xq  = 0.071  0.73%
```

Accuracy and Precision Check

Concentration	= 0.101 g/210L
Lot #	= 12-38-100
Range	= 0.096 - 0.106
Average	= 0.100 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

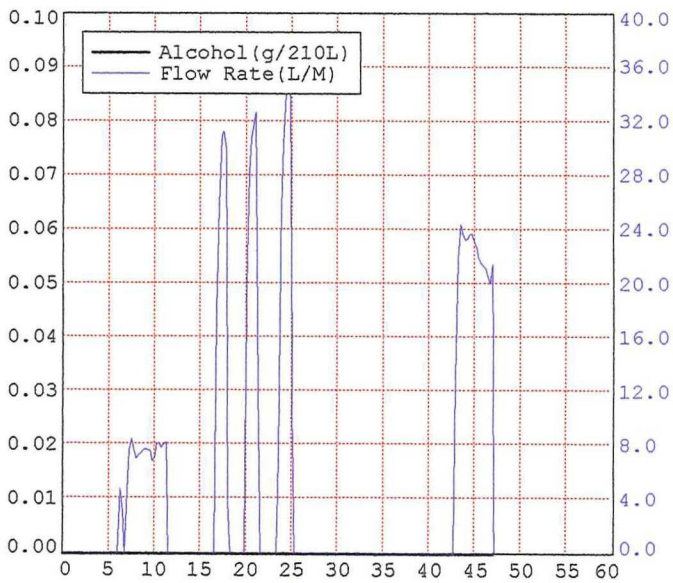

INSTALLATION PASSED

Performed by _____ Date 12/01/2011 12/5/11

Reviewed by _____ Date 12-1-11