INSTALLATION REPORT

DataMaster DMT: 100164
Location: Rutland City PD
Calibration Date: 08/31/2011
Certification Date: 08/31/2011
Installation Date: 12/01/2011
Installed by: STEVEN E HARNOIS

Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.2
Questions: 2.0

TEMPERATURES

Sample Chamber = 48.7°C
Breath Tube    = 42.5°C
Digital Sim    = 33.9°C

SETTINGS
Lamp Voltage   = 1.81 V
Cooler Voltage = 1.71 V
Bias Voltage   = 80 V
Chopper Freq   = 543 Hz

PUMP INFO
Flow Rate = 5.719 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   -0.0585   -0.0555
MIN(V)   -0.0604   -0.0569

FILTER INFO
Filter 1  -0.055  Zero = true
Filter 2   0.142  Zero = true
Filter 3   0.635  Zero = true

CALIBRATION CHECK
Xq  = 0.091  0.58%
```

Accuracy and Precision Check

Concentration = 0.101 g/210L
Lot # = 12-38-100
Range = 0.096 - 0.106
Average = 0.099 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

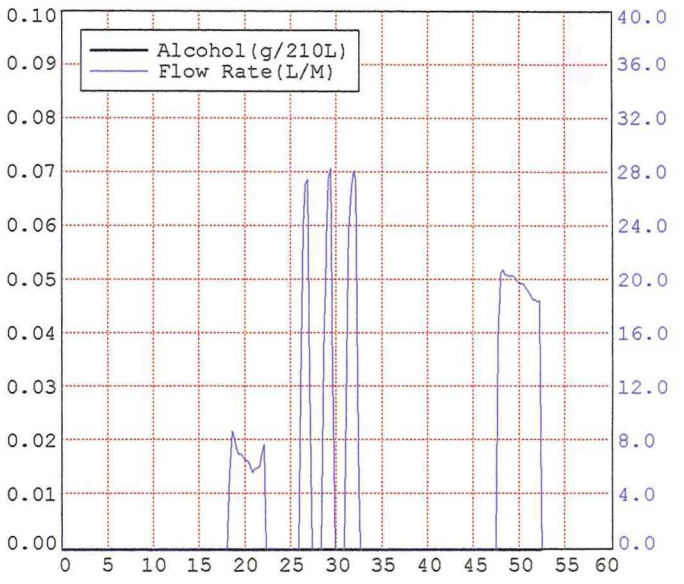

INSTALLATION PASSED

12/5/11

Performed by _____ Date 12/01/2011

Reviewed by _____ Date 12-1-11