

INSTALLATION REPORT

DataMaster DMT: 100141
Location: VERGENNES PD
Calibration Date: 11/01/2011
Certification Date: 11/01/2011
Installation Date: 11/03/2011
Installed By: STEVEN E HARNOIS



Site meets specification in doc P-ALC-210

Diagnostic Results

VERSIONS
DMT 1.04
PIC 2.05
Modem 1.06
Questions 1.00
Reports 1.02

TEMPERATURES
Sample Chamber = 49.03°C
Breath Tube = 48.09°C
Digital Sim = 33.8°C

SETTINGS
Lamp Voltage = 1.73 V
Cooler Voltage = 1.74 V
Bias Voltage = 80.2 V
Chopper Freq = 545.9 Hz

PUMP INFO
Flow Rate = 6.008 L/M

DETECTOR INFO
PUMP ON OFF
MAX(V) 0.0297 0.0313
MIN(V) 0.0283 0.0305

FILTER INFO
Filter 1 0.031 ✓ Zero = true
Filter 2 0.335 Zero = true
Filter 3 0.637 Zero = true

CALIBRATION CHECK
Xq = 0.0788 0.65%

INSTALLATION PASSED

Accuracy and Precision Check


Concentration = 0.100 g/210L
Lot # = 12-32-100
Average = 0.099 g/210L
Std Dev = 0.001

RFI Interference Test

RFI detected

Sample Acceptance Test

Passed

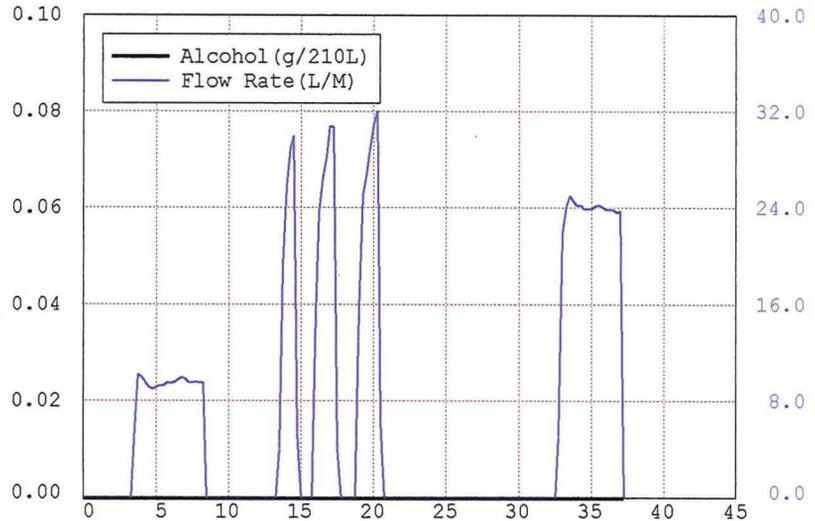

Performed by Steve Harno

Date 11/03/2011

Reviewed by W L J

Date 11-3-11

DMT Serial Number #100141

Page 1 of 1

11/03/2011 09:24