INSTALLATION REPORT

DataMaster DMT: 123306
Location: New Haven VSP
Calibration Date: 12/23/2011
Certification Date: 12/23/2011
Installation Date: 01/12/2012
Installed by: STEVEN E HARNOIS

Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.2
Questions: 2.0

TEMPERATURES

Sample Chamber = 49.0°C
Breath Tube    = 48.1°C
Digital Sim    = 33.9°C

SETTINGS
Lamp Voltage   = 1.66 V
Cooler Voltage = 1.77 V
Bias Voltage   = 80 V
Chopper Freq   = 529 Hz

PUMP INFO
Flow Rate = 4.836 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.0061    0.0116
MIN(V)   0.0051    0.0096

FILTER INFO
Filter 1   0.010  Zero = true
Filter 2   0.499  Zero = true
Filter 3   1.124  Zero = true

CALIBRATION CHECK
Xq  = 0.126  0.00%
```

Accuracy and Precision Check

Concentration	= 0.100 g/210L
Lot #	= 12-45-100
Range	= 0.095 - 0.105
Average	= 0.099 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

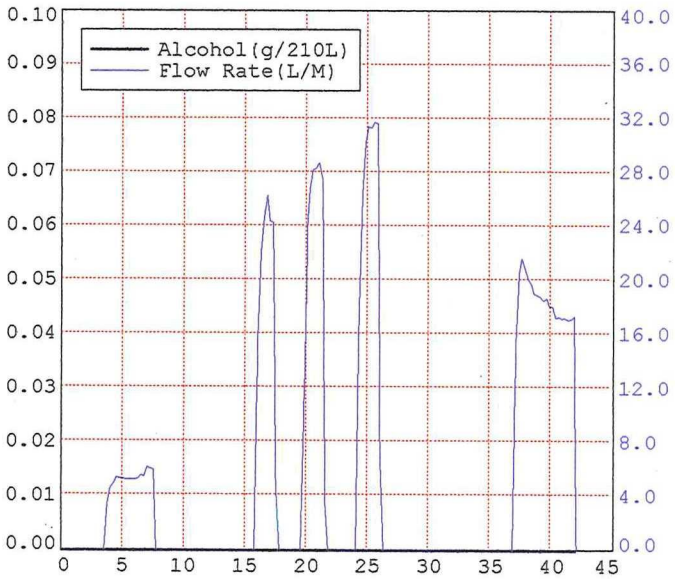

INSTALLATION PASSED

Performed by _____ Date 01/12/2012

Reviewed by _____ Date 1-12-12

Reviewed 01/12/12 JKm