INSTALLATION REPORT

DataMaster DMT: 100150
Location: Bristol PD
Calibration Date: 02/14/2012
Certification Date: 02/15/2012
Installation Date: 02/22/2012
Installed by: STEVEN E HARNOIS

Site meets specification in doc P-ALC-210

Default Options Loaded

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.2
Questions: 2.0

TEMPERATURES

Sample Chamber = 49.0°C
Breath Tube    = 44.0°C
Digital Sim    = 34.2°C

SETTINGS
Lamp Voltage   = 1.60 V
Cooler Voltage = 1.58 V
Bias Voltage   = 80 V
Chopper Freq   = 534 Hz

PUMP INFO
Flow Rate = 5.894 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   -0.0661   -0.0614
MIN(V)   -0.0675   -0.0630

FILTER INFO
Filter 1  -0.061  Zero = true
Filter 2   0.719  Zero = true
Filter 3   0.674  Zero = true

CALIBRATION CHECK
Xq  = 0.084  0.31%
```

Accuracy and Precision Check

Concentration	= 0.100 g/210L
Lot #	= 12-58-100
Range	= 0.095 - 0.105
Average	= 0.099 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

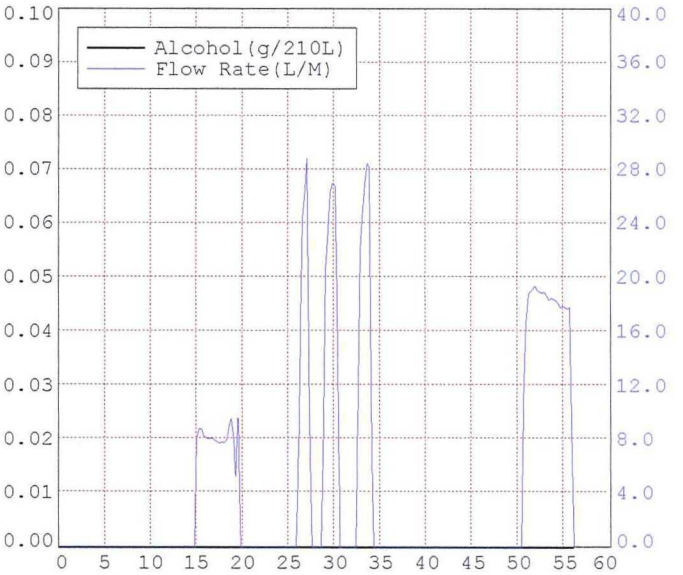

INSTALLATION PASSED

Rev. 2-23-12

Performed by _____ Date 02/22/2012

Reviewed by _____ Date 2/22/12