

ROUTINE PERFORMANCE CHECK REPORT



RECEIVED

FEB 29 2012

Vermont Department of Health Laboratory

DataMaster DMT: 123206
 Location: Middlebury PD
 Calibration Date: 01/03/2012
 Certification Date: 01/04/2012
 Installation Date: 01/12/2012
 RPC Date: 02/27/2012
 Supervisor Name: KEVIN A EMILIO

Diagnostic Results

VERSIONS

DMT: 1.01
 PIC: 2.05
 Modem: 2.2
 Questions: 2.0

TEMPERATURES

Sample Chamber = 48.7°C
 Breath Tube = 44.6°C
 Digital Sim = 33.9°C

SETTINGS

Lamp Voltage = 1.73 V
 Cooler Voltage = 1.77 V
 Bias Voltage = 80 V
 Chopper Freq = 539 Hz

PUMP INFO

Flow Rate = 4.492 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.0982	0.1024
MIN (V)	0.0967	0.1006

FILTER INFO

Filter	Value	Zero
Filter 1	0.101	Zero = true
Filter 2	0.464	Zero = true
Filter 3	1.467	Zero = true

CALIBRATION CHECK

Xq = 0.081 0.11%

Routine Performance Check Passed

Accuracy and Precision Check


Concentration	= 0.100 g/210L
Lot #	= 12-45-100
Range	= 0.095 - 0.105
Average	= 0.100 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

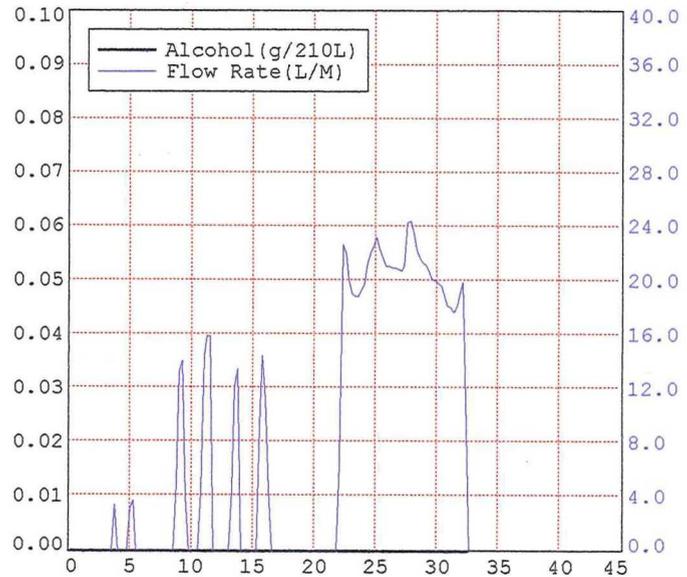

Performed by KE

Date


02/27/2012

Reviewed by Steven Harnois

Date

3/1/12

ROUTINE PERFORMANCE CHECK REPORT

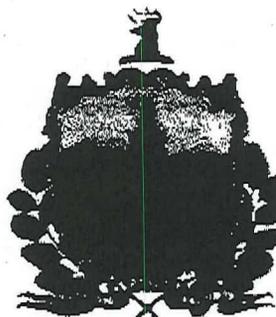

DataMaster DMT: 123206
 Location: Middlebury PD
 Calibration Date: 01/03/2012
 Certification Date: 01/04/2012
 Installation Date: 01/12/2012
 RPC Date: 02/27/2012
 Supervisor Name: KEVIN A EMILIO

Diagnostic Results

VERSIONS

DMT: 1.01
 PIC: 2.05
 Modem: 2.2
 Questions: 2.0

TEMPERATURES

Sample Chamber = 48.7°C
 Breath Tube = 44.6°C
 Digital Sim = 33.9°C

SETTINGS

Lamp Voltage = 1.73 V
 Cooler Voltage = 1.77 V
 Bias Voltage = 80 V
 Chopper Freq = 539 Hz

PUMP INFO

Flow Rate = 4.492 L/M

DETECTOR INFO

PUMP	ON	OFF
MAX (V)	0.0982	0.1024
MIN (V)	0.0967	0.1006

FILTER INFO

Filter	Value	Zero
Filter 1	0.101	Zero = true
Filter 2	0.464	Zero = true
Filter 3	1.467	Zero * true

CALIBRATION CHECK

Xq = 0.081 0.11%

Accuracy and Precision Check


Concentration = 0.100 g/210L
 Lot # = 12-45-100
 Range = 0.095 - 0.105
 Average = 0.100 g/210L
 Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

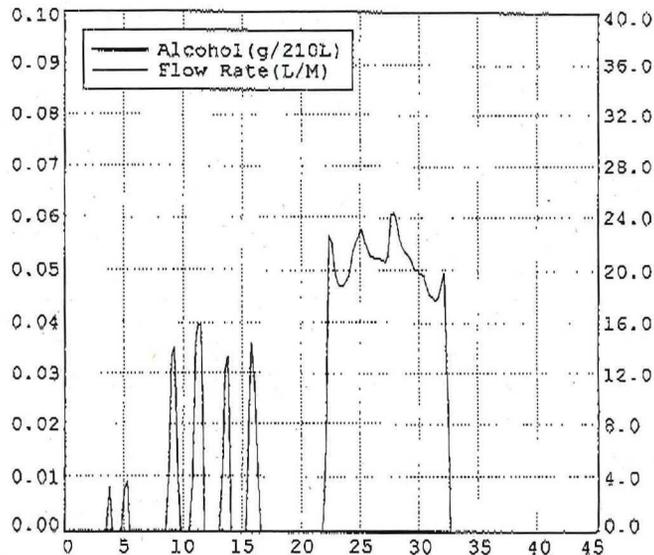

Routine Performance Check Passed

2/29/12

Email Sent Requesting Color Copy SH 3-12-12

Performed by *KEV*

Date 02/27/2012

Reviewed by _____

Date _____



Middlebury Police Department

ONE LUCIUS SHAW LANE, MIDDLEBURY, VERMONT 05753
TELEPHONE (802) 388-3191
FAX (802) 388-4363

Thomas Hanley
Chief of Police

FACSIMILE TRANSMISSION COVER SHEET

TO: Steven Harwood
ATTENTION: "
FAX NUMBER: 802-863-7632
NUMBER OF PAGES (including this cover sheet): 2
FROM: K. Emilio
DATE: 2/27/12 TIME: 1520

2/12 RPC

***** WARNING *****

THE DOCUMENT ACCOMPANYING THIS TELECOPY TRANSMISSION CONTAINS INFORMATION FROM THE MIDDLEBURY POLICE DEPARTMENT, WHICH IS CONFIDENTIAL AND MAY BE LEGALLY PRIVILEGED. THE INFORMATION IS INTENDED ONLY FOR THE USE OF THE INDIVIDUAL OR ENTITY NAMED ON THIS COVER SHEET. IF YOU ARE NOT THE INTENDED RECIPIENT, YOU ARE HEREBY NOTIFIED THAT ANY DISCLOSURE, COPYING, DISTRIBUTION, OR TAKING OF ANY ACTION IN RELIANCE ON THE CONTENTS OF THIS TELECOPIED INFORMATION IS STRICTLY PROHIBITED. IF YOU HAVE RECEIVED THIS TELECOPY IN ERROR, OR IT CANNOT BE DELIVERED TO THE INTENDED RECIPIENT, PLEASE NOTIFY THIS DEPARTMENT AT (802) 388-3191 SO THAT WE CAN ARRANGE RETURN OF THE DOCUMENT.

If this transmission has been disrupted, or all pages not received, please notify the sender at (802) 388-3191.