ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 100150
Location: Bristol PD
Calibration Date: 02/14/2012
Certification Date: 02/15/2012
Installation Date: 09/30/2013
RPC Date: 11/24/2014
Supervisor Name: KEVIN E GIBBS

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.06
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 48.8°C
Breath Tube    = 47.3°C
Digital Sim    = 34.0°C

SETTINGS
Lamp Voltage   = 1.60 V
Cooler Voltage = 1.58 V
Bias Voltage   = 80 V
Chopper Freq   = 546 Hz

PUMP INFO
Flow Rate = 5.555 L/M

DETECTOR INFO
PUMP     ON         OFF
MAX(V)    0.2002     0.2028
MIN(V)    0.1988     0.2014

FILTER INFO
Filter 1   0.203  Zero = true
Filter 2   0.939  Zero = true
Filter 3   0.933  Zero = true

CALIBRATION CHECK
Xq  = 0.084  0.21%
```

Routine Performance Check Passed

Accuracy and Precision Check

Concentration = 0.098 g/210L
Lot # = 14-12-100
Range = 0.093 - 0.103
Average = 0.098 g/210L
Std Dev = 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

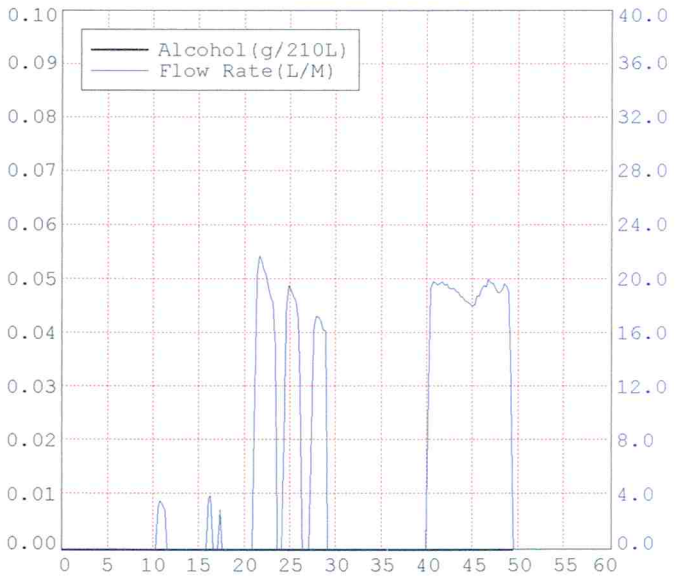

Performed by _____ Date 11/24/2014

Reviewed by _____ Date _____

Breath Record History

Test Date	Test Time	Agency	Operator Name	Alcohol Val. 1	Alcohol Val. 2	Sim. Conc. 1	Sim. Conc. 2	Status Message
05/05/2012	19:49:26	ADDISON COUNTY SHERIFF	DALE BENWAY			0.094		Simulator Out of Range
07/07/2012	02:44:46	BRISTOL PD	GEORGE R CROWE	0.000		0.099		
07/09/2012	21:26:49	Bristol Police Department	JOSHUA L OTEY			0.098		RESPONSE TIMEOUT
07/09/2012	21:32:36	Bristol Police Department	JOSHUA L OTEY	0.209		0.098		
07/22/2012	08:21:49	BRISTOL PD	GEORGE R CROWE	INVALID		0.097		
07/22/2012	08:42:19	BRISTOL PD	GEORGE R CROWE	INVALID		0.097		
07/22/2012	09:02:58	BRISTOL PD	GEORGE R CROWE	0.177		0.097		
09/02/2012	05:44:33	BRISTOL PD	GEORGE R CROWE	0.178		0.096		
09/17/2012	19:21:20	BRISTOL PD	JOSHUA L OTEY	INCOMPLETE		0.095		Pump Error
09/17/2012	19:58:38	BRISTOL PD	JOSHUA L OTEY	INVALID		0.095		
09/17/2012	20:19:25	BRISTOL PD	JOSHUA L OTEY	0.139		0.095	0.094	Simulator Out of Range
10/12/2012	00:34:24	BRISTOL PD	GEORGE R CROWE			0.093		Simulator Out of Range
10/23/2012	20:22:04	Bristol Police	JOSHUA L OTEY			0.093		Simulator Out of Range
10/23/2012	20:25:49	Bristol Police	JOSHUA L OTEY			0.093		Simulator Out of Range
11/20/2012	15:48:29	Bristol Police Department	KEVIN E GIBBS			0.093		Simulator Out of Range
11/20/2012	15:52:09	Bristol Police Department	KEVIN E GIBBS			0.094		Simulator Out of Range
11/20/2012	15:55:52	Bristol Police Department	KEVIN E GIBBS	0.156		0.095		
03/24/2013	01:11:34	BRISTOL PD	JOSHUA L OTEY	0.131		0.095		RESPONSE TIMEOUT
04/20/2013	00:46:33	BRISTOL PD	GEORGE R CROWE			0.093		Simulator Out of Range
05/28/2013	00:04:01	BRISTOL PD	GEORGE R CROWE			0.091		Simulator Out of Range
05/28/2013	00:07:40	BRISTOL PD	GEORGE R CROWE			0.091		Simulator Out of Range
05/28/2013	00:12:06	BRISTOL PD	GEORGE R CROWE			0.091		Simulator Out of Range
08/10/2013	20:23:12	Bristol	JOSHUA L OTEY	REFUSED		0.097		
08/10/2013	20:44:45	BRISTOL PD	JOSHUA L OTEY	0.149		0.097		
10/13/2013	02:24:50	BRISTOL PD	GEORGE R CROWE					Simulator Timed Out
10/13/2013	02:29:14	BRISTOL PD	GEORGE R CROWE					Simulator Timed Out
04/11/2014	22:52:25	NEW HAVEN VSP	JOSEPH T SZAREJKO			0.093		Simulator Out of Range
04/11/2014	22:56:13	NEW HAVEN VSP	JOSEPH T SZAREJKO			0.092		Simulator Out of Range
04/11/2014	23:03:06	NEW HAVEN VSP	JOSEPH T SZAREJKO			0.092		Simulator Out of Range
04/15/2014	21:14:27	BRISTOL PD	GEORGE R CROWE			0.092		Simulator Out of Range
04/18/2014	18:42:12	Bristol PD	KEVIN E GIBBS	0.000		0.097		
04/18/2014	23:23:44	BRISTOL PD	JOSHUA L OTEY	0.082		0.097		
05/14/2014	21:21:14	Bristolo PD	KEVIN E GIBBS	0.197	INCOMPLETE	0.097	0.096	RESPONSE TIMEOUT
05/16/2014	14:11:29	Bristol PD	KEVIN E GIBBS	0.312		0.096		
10/18/2014	22:00:35	BRISTOL PD	JOSHUA L OTEY	0.142		0.094		
10/30/2014	22:40:17	BRISTOL PD	JOSHUA L OTEY	0.120		0.094		
12/27/2014	02:31:49	BRISTOL PD	GEORGE R CROWE	0.153		0.096		

Log On Record History

Test Date	Test Time	Name
02/14/2012	07:53:24	Kirk Kimball
02/14/2012	13:52:44	Kirk Kimball
02/14/2012	14:06:24	Steven Merrill
02/14/2012	14:14:34	Steven Merrill
02/14/2012	14:38:48	Supervisor
02/14/2012	14:43:16	Kirk Kimball
02/14/2012	15:03:29	Steven Merrill
02/14/2012	15:29:05	Steven Merrill
02/15/2012	07:30:52	Kirk Kimball
02/15/2012	08:06:34	Steven Merrill
02/15/2012	08:47:02	Steven Merrill
02/15/2012	15:45:22	Steven Merrill
02/16/2012	07:04:50	Kirk Kimball
02/16/2012	07:19:53	Kirk Kimball
02/16/2012	10:47:42	Steven Merrill
02/16/2012	13:20:22	Steven Merrill
02/17/2012	06:51:36	Kirk Kimball
02/17/2012	07:56:26	Kirk Kimball
02/17/2012	09:42:37	Steven Merrill
02/17/2012	13:15:35	Steven Merrill
02/17/2012	14:40:09	Steven Merrill
02/18/2012	09:08:23	Kirk Kimball
02/22/2012	14:05:20	Steven Harnois
06/27/2012	12:24:16	Supervisor
08/29/2012	12:11:51	Amanda Bolduc
08/29/2012	12:13:57	Amanda Bolduc

Status Record History

Status Date	Status Time	Test Type	Status Message
02/15/2012	15:47:10	Accuracy & Precision Records	Simulator Timed Out
02/17/2012	11:16:52	Accuracy & Precision Records	Blank Error
02/17/2012	15:09:39	Accuracy & Precision Records	Simulator Temperature Too High
05/05/2012	19:50:59	DUI Subject Record	Simulator Out of Range
06/27/2012	13:03:59	RPC Record	RF NOT DETECTED
07/09/2012	21:30:10	DUI Subject Record	RESPONSE TIMEOUT
09/17/2012	19:26:05	DUI Subject Record	Pump Error
09/17/2012	20:25:29	DUI Subject Record	Simulator Out of Range
10/12/2012	00:35:57	DUI Subject Record	Simulator Out of Range
10/23/2012	20:23:43	DUI Subject Record	Simulator Out of Range
10/23/2012	20:27:25	DUI Subject Record	Simulator Out of Range
10/30/2012	12:40:29	RPC Record	ACCURACY AND PRECISION CHECK FAILED
10/30/2012	12:51:21	RPC Record	RF NOT DETECTED
11/20/2012	15:50:05	DUI Subject Record	Simulator Out of Range
11/20/2012	15:53:43	DUI Subject Record	Simulator Out of Range
01/25/2013	13:33:45	APM Record	ACCURACY AND PRECISION CHECK FAILED
03/24/2013	01:16:45	DUI Subject Record	RESPONSE TIMEOUT
04/20/2013	00:48:07	DUI Subject Record	Simulator Out of Range
05/28/2013	00:05:37	DUI Subject Record	Simulator Out of Range
05/28/2013	00:09:16	DUI Subject Record	Simulator Out of Range
05/28/2013	00:13:44	DUI Subject Record	Simulator Out of Range
09/30/2013	11:36:20	Installation Record	ACCURACY AND PRECISION CHECK FAILED
10/13/2013	02:26:56	DUI Subject Record	Simulator Timed Out
10/13/2013	02:31:20	DUI Subject Record	Simulator Timed Out
10/19/2013	22:22:52	RPC Record	ACCURACY AND PRECISION CHECK FAILED
10/20/2013	12:24:12	RPC Record	ACCURACY AND PRECISION CHECK FAILED
10/20/2013	13:07:20	RPC Record	ACCURACY AND PRECISION CHECK FAILED
04/11/2014	22:54:03	DUI Subject Record	Simulator Out of Range
04/11/2014	22:57:45	DUI Subject Record	Simulator Out of Range
04/11/2014	23:04:40	DUI Subject Record	Simulator Out of Range
04/15/2014	21:16:07	DUI Subject Record	Simulator Out of Range
04/18/2014	18:25:07	Solution Change Record	ACCURACY AND PRECISION CHECK FAILED
05/14/2014	21:32:31	DUI Subject Record	RESPONSE TIMEOUT
11/24/2014	16:13:08	RPC Record	Diagnostic Check Failed
11/24/2014	16:16:10	RPC Record	Diagnostic Check Failed
11/24/2014	17:00:10	RPC Record	ACCURACY AND PRECISION CHECK FAILED