DataMaster DMT Monthly Update Check-list

Department/Agency: MIDDLEBURY PD DM serial #: 123206

Date: 07, 08, 14

	Provided	None this month
Operators Logbook	☐	☑
Maintenance Logbook	☑	☐
Breath Summary Report	☑	☐
Status Summary Report	☑	☐
Calibration Report	☐	☑
Certification Report	☐	☑
Installation Report	☐	☑
Annual Preventative Maintenance	☐	☑
Routine Performance Check	☑	☐
Simulator Solution Change	☐	☑
Other Reports	☐	☑

List other report type and date:

MONTHLY DMT REPORT FOR JUNE 2014

Breath Record History

Test Date	Test Time	Agency	Operator Name	Alcohol Val. 1	Alcohol Val. 2	Sim. Conc. 1	Sim. Conc. 2	Status Message
06/08/2014	03:22:55	MIDDLEBURY PD	VEGAR BOE	REFUSED		0.095		
06/14/2014	01:14:53	MIDDLEBURY PD	VEGAR BOE	0.139		0.095		Blank Error
06/14/2014	01:19:31	MIDDLEBURY PD	VEGAR BOE	0.150	0.149	0.095	0.096	
06/22/2014	03:01:56	MIDDLEBURY PD	VEGAR BOE	0.163		0.095		
06/25/2014	15:59:16	MIDDLEBURY PD	KEVIN A EMILIO	INCOMPLETE	0.196	0.094		
06/29/2014	02:20:28	MIDDLEBURY PD	VEGAR BOE	0.198		0.099		

Status Record History

Status Date	Status Time	Test Type	Status Message
06/14/2014	01:17:52	DUI Subject Record	Blank Error

ROUTINE PERFORMANCE CHECK REPORT

DataMaster DMT: 123206
Location: Middlebury PD
Calibration Date: 01/03/2012
Certification Date: 01/04/2012
Installation Date: 01/12/2012
RPC Date: 06/27/2014
Supervisor Name: KEVIN A EMILIO

Diagnostic Results

```
VERSIONS
DMT: 1.01
PIC: 2.05
Modem: 2.4
Questions: 2.1

TEMPERATURES

Sample Chamber = 49.0°C
Breath Tube    = 46.5°C
Digital Sim    = 33.9°C

SETTINGS
Lamp Voltage   = 1.73 V
Cooler Voltage = 1.78 V
Bias Voltage   = 80 V
Chopper Freq   = 543 Hz

PUMP INFO
Flow Rate = 4.466 L/M

DETECTOR INFO
PUMP     ON        OFF
MAX(V)   0.3494    0.3531
MIN(V)   0.3476    0.3516

FILTER INFO
Filter 1   0.353  Zero = true
Filter 2   0.704  Zero = true
Filter 3   1.640  Zero = true

CALIBRATION CHECK
Xq  = 0.080  0.54%
```

Routine Performance Check Passed

Accuracy and Precision Check

Concentration	= 0.098 g/210L
Lot #	= 14-05-100
Range	= 0.093 - 0.103
Average	= 0.099 g/210L
Std Dev	= 0.0000

RF Detection Test

Passed

Sample Acceptance Test

Passed

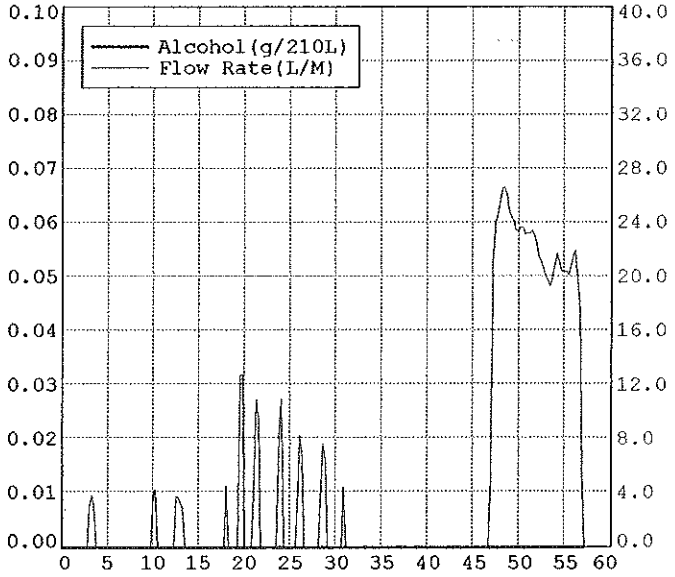

Performed by _____ Date 06/27/2014

Reviewed by _____ Date _____

DATAMASTER DMT MAINTENANCE LOG

MIDDLEBURY PD
Department/Agency

123206
DataMaster DMT Serial Number

DATE	TYPE OF SERVICE PERFORMED	PERFORMED BY (Name and Title)
2/11/14	**DataMaster Simulator Solution** Lot # 13-16-100 EtOHaq Conc: 0.099 Range: 0.094 - 0.104 Preparation Date: 9/26/2013 Expires: 09/26/2014 OPENED: 2-11-14 [Change Place Label Here] RPC Conducted	KEVIN A. EMILIO DMT SUPV.
6/27/14	**DataMaster Simulator Solution** Lot # 14-05-100 EtOHaq Conc: 0.098 Range: 0.093 - 0.103 Preparation Date: 6/19/2014 Expires: 6/19/2015 OPENED: 6-27-14 [Change Place Label Here] RPC Conducted	Kevin A. Emilio DMT SUPV.
	[For RPC or Simulator Solution Change Place Label Here]	
	[For RPC or Simulator Solution Change Place Label Here]	

ALC 803 REV 03 08/2011